

EFFECTIVE HUMIDIFICATION. EFFECTIVE PROTECTION.


DAR™ Filter HMEs



A heat and moisture exchanger (HME) captures heat and water vapor from a patient's exhaled air. It then adds that heat and moisture to the patient's inspired air, providing humidification.

A recently published study showed that of 48 filters and HMEs tested, 3 DAR™ filter HMEs ranked in the top 10 for humidity output.¹


Measured absolute humidity in independent published testing

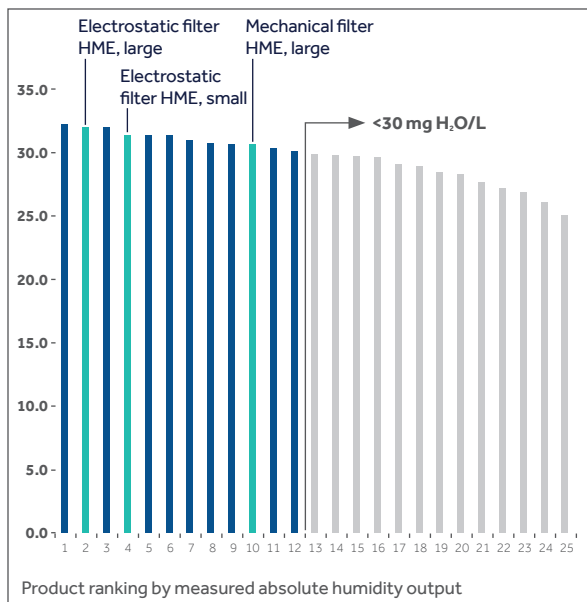

Source: Lellouche et al¹



Electrostatic filter HME, large



Mechanical filter HME, large



Electrostatic filter HME, small



Electrostatic filter HME, small, angled port



Pediatric electrostatic filter HME, small



Infant-pediatric electrostatic filter, small

Medtronic
Further. Together

ELECTROSTATIC FILTER HMEs

	Large	Small	Small, Angled Port	Pediatric	Infant-Pediatric
Catalog number	352U5805	352U5877	352U5996	355U5430	355U5427
Quantity/box	50	50	50	50	50
Recommended tidal volume	300-1500 mL	150-1200 mL	150-1200 mL	75-300 mL	30-100 mL
Moisture output					
Vt 50 mL	---	---	---	---	28 mg H ₂ O/L ²
Vt 250 mL	33.9 mg H ₂ O/L ²	34.4 mg H ₂ O/L ⁴	34.4 mg H ₂ O/L ⁴	31 mg H ₂ O/L ²	---
Vt 500 mL	33.3 mg H ₂ O/L ²	33.6 mg H ₂ O/L ²	33.6 mg H ₂ O/L ²	---	---
Vt 1000 mL	32.4 mg H ₂ O/L ²	32.9 mg H ₂ O/L ⁴	32.9 mg H ₂ O/L ⁴	---	---
Moisture loss*	6 mg H ₂ O/L at Vt 500 mL	6 mg H ₂ O/L at Vt 500 mL ⁴	6 mg H ₂ O/L at Vt 500 mL	6 mg H ₂ O/L at Vt 75 mL	NA
Resistance to flow before use (ISO 9360)					
5 L/min	---	---	---	---	0.6 cm H ₂ O
15 L/min	---	---	---	1.4 cm H ₂ O	2.5 cm H ₂ O
30 L/min	1.0 cm H ₂ O	1.2 cm H ₂ O	1.2 cm H ₂ O	3.0 cm H ₂ O	---
60 L/min	2.1 cm H ₂ O	2.8 cm H ₂ O	2.9 cm H ₂ O	---	---
90 L/min	3.7 cm H ₂ O	4.8 cm H ₂ O	5.2 cm H ₂ O	---	---
Filtration efficiency					
Bacterial	≥99.9999%	≥99.9998%	≥99.9998%	≥99.999%	≥99.999%
Viral	≥99.998%	>99.999%	>99.999%	≥99.99%	≥99.99%
NaCl¹	≥99.623%	≥98.352% ⁶	≥98.352% ⁶	≥96.263%	≥94.186%
Internal volume	93 mL	51 mL	61 mL	29 mL	10 mL
Weight (approx.)	48 g	28 g	29 g	21 g	9 g
Type of filtration	Electrostatic	Electrostatic	Electrostatic	Electrostatic	Electrostatic

DAR™ filter HMEs have been tested against microbes as small as 0.02 µ.

MECHANICAL FILTER HMEs

	Large
Catalog number	354U5876
Quantity/box	50
Recommended tidal volume	300-1500 mL
Moisture output	
Vt 50 mL	---
Vt 250 mL	34.7 mg H ₂ O/L ⁵
Vt 500 mL	34.1 mg H ₂ O/L ²
Vt 1000 mL	33.4 mg H ₂ O/L ⁵
Moisture loss*	5 mg H ₂ O/L at Vt 500 mL ⁵
Resistance to flow before use (ISO 9360)	
5 L/min	---
15 L/min	---
30 L/min	1.1 cm H ₂ O
60 L/min	2.5 cm H ₂ O
90 L/min	4.2 cm H ₂ O
Filtration efficiency:	
Bacterial	≥99.9999%
Viral	≥99.9999%
NaCl⁴	≥99.764%
Internal volume	96 mL
Weight (approx.)	49 g
Type of filtration	Mechanical

DAR™ filter HMEs have been tested against microbes as small as 0.02 µ.

*Internal testing Mirandola (various 2005-2008).

- Lellouche F, Taillé S, Lefrançois F, et al. Humidification performance of 48 passive airway humidifiers: comparison with manufacturer data. *Chest*. 2009;135(2):276-286.
- MHRA. Evaluation no. 04005: Breathing system filters, an assessment of 104 breathing system filters. March 2004.
- Nelson Laboratories Inc. Sodium chloride aerosol testing of breathing system filters (BSF). Lab.No. 399951A.1 Amended. January 2008.
- TIM, Technologie-Institut Medizin GmbH - Universitätsklinikum Göttingen, Germany. HME-Test Report 2008/22 DAR Hygrobac "S". July 2008.
- TIM, Technologie-Institut Medizin GmbH - Universitätsklinikum Göttingen, Germany. HME-Test. Report 2009/04 DAR Hygroster. May 2009.
- Nelson Laboratories Inc. Sodium chloride aerosol testing of breathing system filters (BSF). Lab.No. 717597. November 2013.

© 2016, 2019 Medtronic. All rights reserved. Medtronic, Medtronic logo and Further Together are trademarks of Medtronic. All other brands are trademarks of a Medtronic company. 10/2019-16-AW-0031(1)-[WF#3593979]