

AUTOMATED ENZYME IMMUNOASSAY SYSTEM

AIA-360

Operator's Manual

Revision 18

REF

0019945

Automated Enzyme Immunoassay System AIA-360

Thank you for purchasing the AUTOMATED ENZYME IMMUNOASSAY SYSTEM AIA-360.

You are recommended to read carefully and familiarize yourselves with the information provided in this manual to ensure safe and correct operation of the system.

TOSOH CORPORATION
BIOSCIENCE DIVISION

Date of publication 04/2025

Version Overview Operator's Manual AIA-360

Version	Date	Amendments
1	01/2007	Original manual
2 -5		Only applied in Japan
6	05/2010	See overview
7		Only applied in Japan
8	12/2010	See overview
9	04/2011	No critical changes
10	09/2015	See overview
11-13		Only applied in Japan
14	12/2018	See overview
14.1	05/2022	See overview
15-17	03/2024	See overview
18	04/2025	See overview

Date	Chapter	Paragraphs
04/2025	1	1.5
	2	2.5
	4	4.2.3
	5	5.1.1 - 5.1.2
		5.2.1 – 5.2.2
	6	6.3
		6.4.1
		6.4.3
	7	7.2.2
	9	9.1
		9.5
	10	10.2.1
		10.5
		10.5.1
	11	11.1 – 11.2
	12	A2
	Address	Addresses
03/2024	Safety Precautions	Caution (III) Additional Precautions (2)
	1	1.4
	2	2.2 - 2.3
		2.5
	3	3.1
	4	4.1
		4.2.3
	5	5.1.2
	6	6.2
		6.4.2
	7	7.1.1
		7.2.2
	9	9.1
	Address	Addresses
05/2022	1	1.1

Date	Chapter	Paragraphs
12/2018	Safety Precautions	Warning (V) Additional Precautions (3)
	1	1.1
		1.2
		1.5
	2	2.5
	3	3.3
		3.5
	4	4.1
		4.2.0
		4.2.3
	7	7.1.1
	8	8.1
	10	10.1.2
		10.2.1
		10.6
	11	11.1
09/2015	3	3.0
		3.6

Preface

It is recommended that you read carefully and familiarize yourselves with the following safety precautions in order to ensure safe and correct operation of the AIA-360 analyzer. The information displayed with the "Warning" and "Caution" signs in this manual is provided for the purposes defined below.



Warning

Indicates a hazard with a medium level of risk which, if not avoided, could result in death or serious injury



Caution

Indicates a hazard with a low level of risk which, if not avoided, could result in minor or moderate injury

Precautions for Installation



Warning

- **Connect System to Suitable Power Source**
 - Make sure to connect the AIA-360 analyzer to a power source that has ample capacity and is free of significant voltage fluctuations.
 - Power sources with insufficient capacity or significant fluctuations in voltage pose a potential fire hazard.
- **Carefully Check Ground Connections**
 - Failure to properly ground the system is a potential source of electrical shock.
 - Make sure to connect the system to a three-pronged power socket.
 - Grounding the system helps to prevent system malfunctions due to noise as well as prevent electrical shock.
 - Do not connect the system ground line to gas pipes, water pipes, lightning rod lines or the telephone system ground line.
 - Gas pipes can ignite fires and cause explosions
 - Water pipes are not an effective ground
 - Lightning rods and telephone lines are a potential source of danger when lightning strikes



Caution

- **Select Installation Site with Care**
 - Refer to section “System Installation” in this manual and select a suitable site for installation of the AIA-360 system. Always contact Tosoh local representatives whenever installing or moving the AIA-360 system.
- **Avoid Altering Power Cables, Using Under-Capacity Extensions and Branch Connecting from Power Outlets**
 - These are potential sources of electrical shock or even fire.
 - Always select extension cables that have sufficient capacity and a ground line.
- **Confirm Plug is Free of Dust or Dirt and Insert Firmly Into Socket**
 - Make sure to remove and inspect the power plug several times a year.
 - Contamination from dust or foreign matter, failure to fully insert into socket or a loose socket may result in electrical shock or even fire.

Precautions for Use



Warning

- **Handling Biohazards With Care**
 - Only personnel with sufficient knowledge of immunological assay techniques and the procedures for handling infectious waste materials should be allowed to operate the AIA-360 system.
 - There is always the possibility that human sera have been contaminated with infectious agents. Mistakes in system operation and handling of such materials can transmit infectious agents to personnel in the general vicinity, as well as to the system operator. It is recommended that all specimens be handled with the utmost care and that the proper protective gear (goggles, gloves, masks etc.) be used at all times during maintenance procedures.
 - All specimen containers, including used reagent cups, reagent bottles, sample cups and waste fluids, have been exposed to human sera. It is recommended that proper protective gear (goggles, gloves, masks etc.) be worn at all times and that waste materials be disposed of in accordance with your area's directive and the relevant laws and regulations in order to protect all personnel in the general operating vicinity and the surrounding environment.
- **Avoid Opening Covers or Panels During Assay Operations**
 - Opening covers or panels during operation may result in personal injury, such as lacerations or even the severing of fingers or hands if they are caught in such moving parts such as the dispense arm.



Caution

- **Operate Only in Accordance with Procedures Described in the Manual**
 - Attempts to operate the AIA-360 using procedures not specified in this manual may affect the integrity of assay results and cause system malfunction.
- **Preventing Leakage of Fluids**
 - Leakages of assay solutions and wash solutions are potential sources of corrosion, electrical shock or even fire.
 - When fluid leakage is discovered, immediately shut down system operation and remove the power plug. It is recommended that proper protective wear (goggles, gloves, masks etc.) be worn at all times when cleaning up the leakage and inspecting and repairing the tubing connections that may be the source of the leak.
 - Should the system continue to leak, contact the nearest Tosoh local representatives.
- **Immediately Shut Down System and Remove Power Plug When Signs of Malfunction (Burnt Odours, Etc.) Appear. Contact the Nearest Tosoh local representatives.**
 - Continuing to operate the system while it is malfunctioning may result in electrical shock and even fire.
- **Avoid Opening Covers or Panels and Inserting Fingers or Rods into Operating Mechanisms.**
 - The interior of the system is comprised of motor driven components operating at high speeds. Foreign objects or fingers and hands can easily be caught in the mechanisms, resulting in personal injury.
- **Keep Covers and Doors Closed During Operation**
 - Keep all covers and doors firmly closed during operation. The interior of the AIA-360 contains various moving parts, high-temperature components and high-voltage circuitry. Fingers and hands can easily get pinched or tangled in the mechanisms, resulting in lacerations, burns and electrical shock.
 - Special precautions must be taken when opening doors to replenish supplies of reagents and sample cups during system operation.
- **Avoid Stopping and Starting System by Simply Inserting and Removing the Power Plug**
 - This may cause electrical shocks or even fires.
 - Whenever shutting down the system, press the power supply switch located at the rear left of the system.
- **Avoid Damaging the Power Supply Cable**
 - Excessive pulling and bending or anchoring the cable into place may damage it, resulting in electrical shock or even fire.
 - Always take firm hold of the plug when removing the power cable.
- **Do Not Replace Fuses Yourself**
 - Always contact the nearest Tosoh local representatives when replacing the fuses installed on the various system circuit boards. Do not attempt to replace fuses yourself.
 - Burnt out fuses can indicate failures in electrical circuits caused by fluid leakage. Thus it is important to contact Tosoh local representatives.



Caution

- **Avoid Touching System Parts with Wet Hands**
 - Touching certain system components may result in electrical shock.
- **Use Only Trained Maintenance Personnel**
 - Maintenance work must be performed by personnel with proper knowledge of system maintenance procedures and equipped with the proper protective gear (goggles, gloves, masks etc.). Physical injury incurred during maintenance can result in infection from specimens. Therefore, it is important that maintenance personnel perform their work in accordance with procedures outlined in this manual and only after they have received sufficient training in maintenance procedures.
 - Feel free to contact Tosoh local representatives for information on maintenance procedures.
- **Properly Disposing of Waste Materials**
 - Take appropriate steps to separate all used materials from assay operations, including reagent cups, reagent bottles, sample cups, specimen containers and waste fluids, according to the type of waste, and dispose of them in accordance with designated procedure. Always wear protective gloves to avoid direct contact with such materials. Waste materials must be disposed of in accordance with your area's directive and the relevant laws and regulations in order to protect all personnel in the general system vicinity and the surrounding environment.
- **Always Wear Protective Gear**
 - Make sure to wear the required protective gear (goggles, gloves, masks etc.) to prevent infection when working with specimens, waste fluids and the accessories used for system calibration.
- **Place Fluid Containers in Their Designated Locations**
 - Placing solution containers randomly in the main unit may result in spillage causing short-circuits that will damage electrical insulation and result in electrical shock.
- **Inspect all specimens for air bubbles and foaming. Remove any air bubbles before analysis.**
 - The liquid surface detection automatically performed on every specimen by the instrument is susceptible to bubbles or foaming. The instrument may detect the bubble as the liquid surface.
Do not run samples which contain bubbles or foam. Make sure to remove any air bubbles before analysis regardless of their size.
- **Use Only Tosoh Designated Components**
 - Use only those accessories and expendables (supplies) listed in the Maintenance Accessories and Expendables section.



Warning



- **At system shutdown, replace the substrate solution remaining in the substrate line with substrate replacement solution (70% ethanol or 70% isopropyl alcohol).**
 - If the substrate solution remains in the substrate line for a long time, it may precipitate. Precipitation in the substrate line may clog the substrate line. Replacement of the substrate solution with distilled water may cause contamination of the substrate line and raise the substrate background.
Make sure to use the substrate replacement solution (70% ethanol or 70% isopropyl alcohol) at system shutdown.
- **Avoid Placing any Source of Flame Near the Substrate Compartment**
 - It is important not to place any sources of flame near the Substrate compartment, as the Substrate line contains 70% ethanol or 70% isopropyl alcohol at the end of an assay operation.
- **Avoid Opening the Specimen Door During STAT (Priority) Sampling**
 - When the STAT door lamp is red it indicates a sampling operation is in progress. Forcing the door open will damage the sampling nozzle and affect the integrity of assay results.

Removal of equipment from use for repair or disposal

- **- Contact the authorized representative**
 - Blood to be tested might have been infected by pathogens. Misconduct on repair or disposal may bring infection to the operator or others working together. In the case of repairing and disposing, please contact the authorized representative.

Additional Precautions

- **Locations of "Warning" and "Caution" Labels**
 - Warning labels are provided at various locations on the AIA-360 system. Read these carefully to ensure safe system operation.

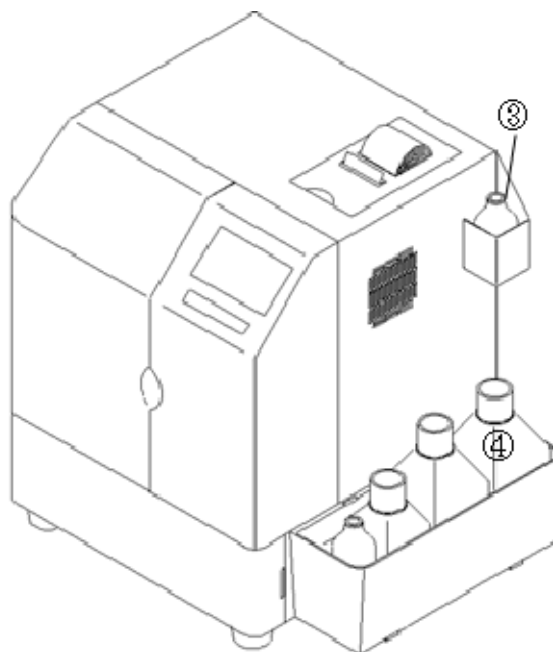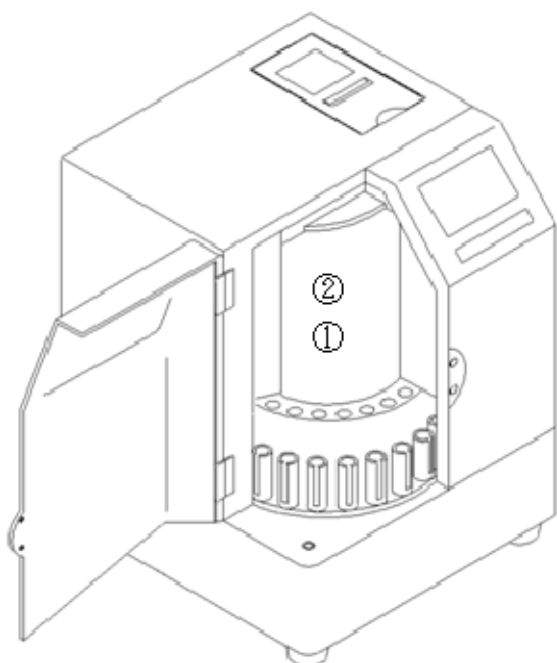

(1) Specimen Loading Location Warning Label



A red lamp comes on 10 seconds prior to start of rotation. Avoid adding or removing specimens or reagents when lamp is flashing, as hands or fingers may get caught in the mechanisms.

(2) Uncap Primary Tubes Warning Label



Please be sure to remove the cap of the primary tubes before placing on the carousel.
Operation will damage parts in the AIA-360 when caps are not removed from the primary tubes.

(3) Substrate Bottle Compartment Warning Label



It is important not to place any sources of flame near the substrate compartment, as the substrate line is composed of 70% ethanol or 70% isopropyl alcohol at the end of an assay operation and there is danger it may catch fire.

(4) Waste Bottle and Contaminated Sera Caution Label



Note that the waste bottles are contaminated from sampled specimen.

It is recommended that proper protective gear (gloves, etc.) be worn at all times when handling waste materials in an effort to prevent contamination.

- Contact Tosoh local representatives if the Warning or Caution labels become difficult to read due to peeling or becoming dirty. Replacement labels will be sent.
- Always store this manual in a safe and convenient place and make sure that it is passed on to any new person in charge.

Always Have Servicing Done by Tosoh Personnel

- Attempts to disassemble, repair or modify the AIA-360 yourself may result in electrical shocks and even fires.

TOSOH CORPORATION
BIOSCIENCE DIVISION


How to Use This Manual

This system Operator's Manual is designed to ensure you will have the information you need to use and operate the AIA-360 system safely and correctly.

The AIA-360 manual is organized according to the layout shown below. Use this as a reference when reading this manual.

Section Headings

Sections are divided into to 3 subsections.

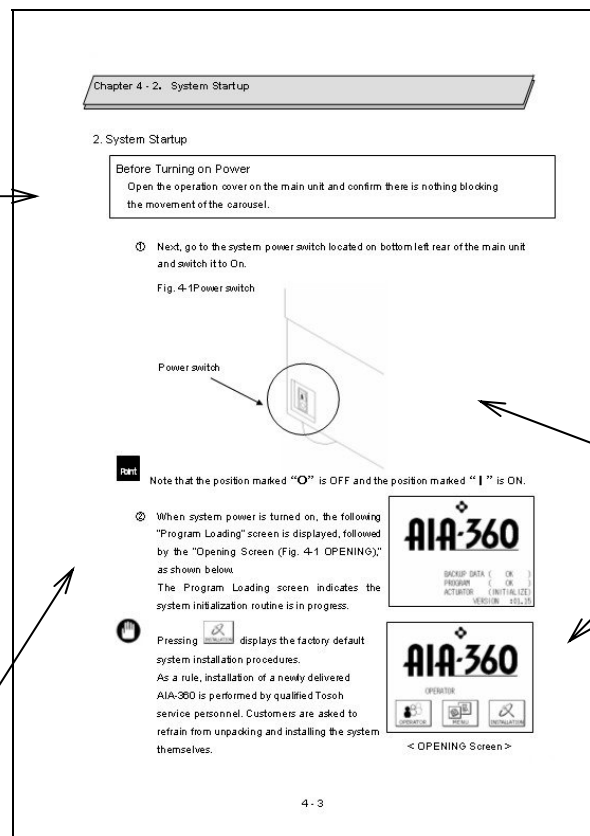

Illustrations and Menu Screens

Combine with text to provide precise explanations.

Page

Numbering is organized by chapter



Key Points provide helpful hints for mastering system operation.



Stop signs warn for potential operational mistakes.

Contents

Chapter 1: Introduction	1-1
1.1. Intended Use	1-1
1.2. Assay Principles	1-1
1.3. System Outline	1-3
1.4. Specifications.....	1-5
1.5. Checking Packing Box Content.....	1-6
[Composition of the seven parts before change (level sensor lead terminal: plug socket type)]	1-8
[Composition of the seven parts after change (level sensor lead terminal: screw type)]	1-9
Chapter 2: Installation	2-1
2.1. Operating Environment.....	2-1
2.2. Environment of transportation and storage	2-1
2.3. Installation Environment	2-2
2.4. Space Required for Installation	2-4
2.5. Installation Procedure	2-5
Connecting Tubing.....	2-5
Connecting Level Sensor Lead Wire (Before Change)	2-7
Connecting Level Sensor Lead Wire 2 (After Change)	2-8
Installing Printer Paper	2-9
Installing Enzyme Substrate Fluid	2-11
2.6. Power Supply.....	2-13
Chapter 3: Name of Parts and Functions on Main Unit	3-1
3.1. Display and Operation Panel.....	3-2
3.2. Carousel	3-3
3.3. Substrate Compartment	3-4
3.4. Printer Unit.....	3-4
3.5. Bottle Tray.....	3-4
3.6. External Recording Media Slot.....	3-4
Chapter 4: Preparing System for Assay Operations	4-1
4.0. Introduction	4-1
4.1. Prior to Commencing Operation	4-2
4.2. System Start-up	4-3
4.2.0. System Start-up	4-3
4.2.1. Confirming/Selecting Operator Name	4-5
4.2.2. Confirming Enzyme Substrate Solution Level.....	4-7
4.2.3. DAILY CHECK.....	4-8
In the Event of Errors.....	4-10
When Starting Assay Before Daily Check is Completed Successfully	4-12
Chapter 5: Calibration.....	5-1
5.0. Introduction	5-1
5.1. Generating Calibration Curves	5-2
5.1.1. Calibration Requests.....	5-2
Procedures	5-2
Changing Concentration.....	5-3
5.1.2. Performing Calibration	5-5

Errors	5-6
5.2. Reviewing/Updating New Calibration Curves.....	5-8
5.2.1. Calibration Review	5-8
Procedures	5-8
To Sort the RATE Values	5-9
5.2.2. Verifying Calibration Curves.....	5-11
Procedures	5-11
Chapter 6: Assay Procedures	6-1
6.0. Introduction	6-1
6.1. Registering Assay Requests.....	6-2
6.2. Registering Sample ID.....	6-3
6.2.1. Entering a sample ID.....	6-3
6.3. Commencing Assay Operations	6-6
Test Tube (sample cup) and Reagent Cup Loading Procedure	6-6
6.4. Assay Results	6-12
6.4.1. External Output of Assay Results	6-12
6.4.2. Printing Assay Results	6-13
6.4.3. Recalculating Assay Results	6-15
Chapter 7: Error Messages and Flags	7-1
7.1. List of Error Messages.....	7-1
7.1.1. Error Message Lists	7-1
7.2. List of Flags	7-12
7.2.1. Flag lists	7-12
7.2.2. Detailed Descriptions of Flags and Actions.....	7-13
7.2.3. Meanings of Daily Check Flags and Actions.....	7-17
Chapter 8: Shut Down Operation (Shut Down Menu)	8-1
8.0. Introduction	8-1
8.1. Shut Down Operation (Shut Down Menu)	8-2
Chapter 9: Other Functions in SPECIAL MENU.....	9-1
9.1. MAINTe (Maintenance Tool)	9-2
9.2. Communications (RS232C Transmission Parameter Settings)	9-6
9.3. DATE/TIME (Time and Date Settings).....	9-7
9.4. OPERATOR (Registering and Changing).....	9-7
9.5. TEST FILE (of Analyte parameters)	9-8
9.6. BCR PARAM (Detailed Barcode Settings)	9-10
9.7. SYSTEM SPEC. (System Operation Settings).....	9-13
Chapter 10: Maintenance Procedures	10-1
10.1. Daily Maintenance Procedures.....	10-1
10.1.1. System Start-up	10-1
10.1.2. System Shutdown	10-1
10.2. Weekly Maintenance Procedures.....	10-1
10.2.1. Substrate Line	10-1
10.3. Monthly Maintenance Procedures.....	10-2
10.3.1. Updating Calibration Curves	10-2
10.4. Three-month Maintenance Procedures.....	10-2
10.4.1. Diluent and Wash Solution Bottles	10-2
10.5. Six-Month Cycle Maintenance Procedures	10-3
10.5.1. Diluent and Wash Lines	10-3
10.5.2. Replacing Filters for Diluent and Wash Solution Bottles.....	10-3

10.6. If AIA-360 Becomes Dirty	10-4
Chapter 11: Consumable Supplies/Optional Parts.....	11-1
11.1. Consumable Supplies.....	11-1
11.2. Optional Parts	11-2
Before change (plug socket type).....	11-2
After change (screw type).....	11-3
Chapter 12: Appendix	12-1
A. Barcode Label Specifications and Precautions for Use	12-1
A.1. Barcode Label Specifications	12-1
A.2. Barcode Effective Read Range	12-1
A.3. Maximum Number of Readable Barcode Digits	12-2
A.4. Loading Test Tubes with Barcode Labels	12-3
B. RS232C Transmission	12-4
B.1. Transmission Specifications	12-4
B.2. Pin Assignment	12-5

Chapter 1: Introduction

Thank you for purchasing the AUTOMATED ENZYME IMMUNOASSAY SYSTEM AIA-360.

This operator's manual provides a detailed description of the system configuration and operating procedures for the AIA-360. You are recommended to read carefully and familiarize yourselves with the information provided in this manual before commencing operation of the system.

1.1. Intended Use

The AUTOMATED ENZYME IMMUNOASSAY SYSTEM AIA-360 is an automated analyser that measures a variety of substances in serum, plasma, and urine using the AIA-PACK reagent series. The AIA-360 is for in vitro diagnostic use by healthcare professionals only.

A notice to the user:

Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the regulatory authority (e.g. EU competent authorities) in the country where the user and/or patient is established.

1.2. Assay Principles

The AIA-360 is capable of performing two methods of immunoassay: an immunoenzymetric (IEMA) or sandwich immunoassay and a competitive binding (EIA) immunoassay.

An antigen-antibody reaction begins by combining a patient sample, control, or calibrator with a diluent in an immunoreaction test cup from the AIA-PACK reagent series. In the IEMA assay, during the incubation period, the antibodies attach to two distinct epitopes on the antigen being measured forming a sandwich. In the EIA assay, during incubation, antigen in the patient sample competes with enzyme labelled antigen for a limited number of antibody binding sites. In all methods, specimens are incubated at 37 °C with antibody bound to the surface of magnetic beads. Separation of the bound antibody from the free antibody is achieved by washing the beads with a wash solution that removes any unbound conjugates. After washing, a substrate, 4-methylumbelliferyl phosphate (4- MUP), is added to the test cup. The remaining enzyme activity on the solid phase (magnetic beads) is then measured using fluorescent rate method. Figure 1.1a illustrates the reaction scheme used on the AIA-360. Figure 1.1b illustrates the Assay Principles used on the AIA-360.

1.2. Assay Principles

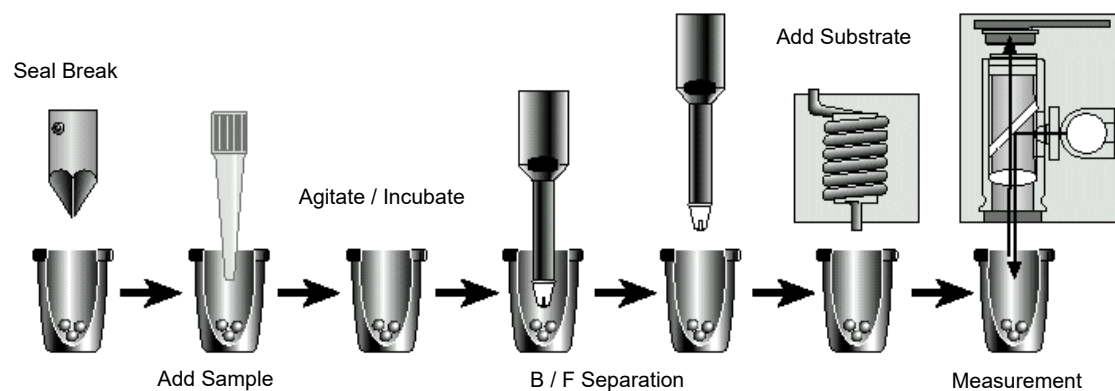


Figure 1.1a AIA-Systems Reaction Scheme

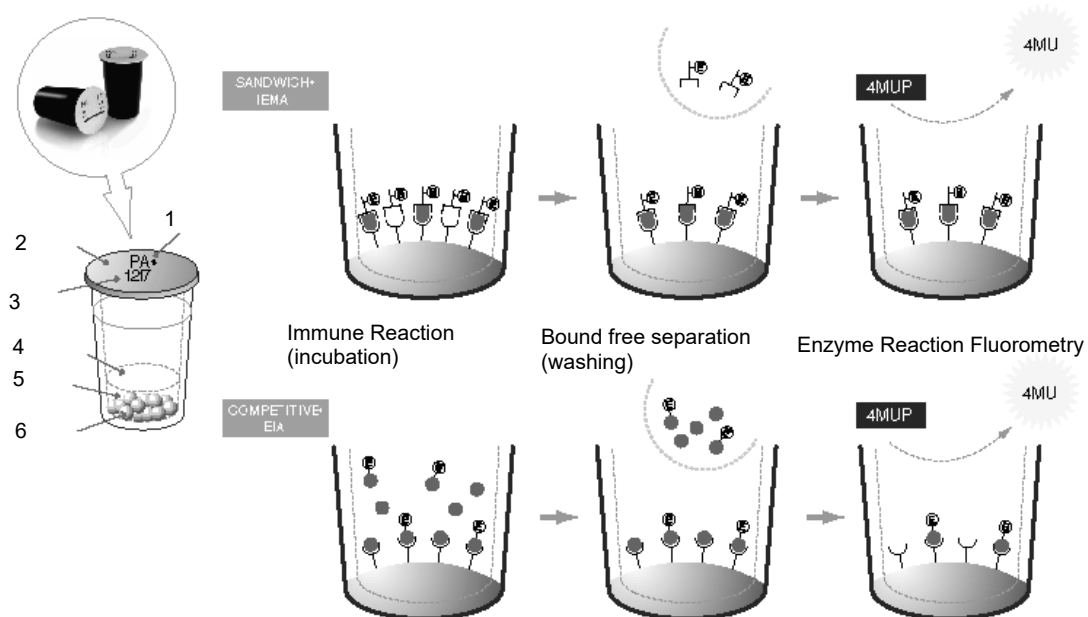



Figure 1.1b AIA-Systems Assay Principles

- (1) Analyte Name
- (2) Aluminium Topseal
- (3) Analyte code & Lot No.
- (4) Enzyme labelled antibody/antigen
- (5) Immobilised antibody
- (6) Magnetic beads

1.3. System Outline

The AIA-360 is designed with a very compact footprint, enabling it to serve as a tabletop unit. While the specimens and reagents used with the AIA-360 must be manually prepared, after sample loading, all processes prior to the assay results and system output are fully automated. The system is capable of performing up to 36 tests per hour. The first test results appear approximately 20 minutes after the assay operation commences. New assay operations can be added, even after assaying has begun. Up to four assay operations can be performed for each specimen.


Fig. 1-1 Overview of Main Unit

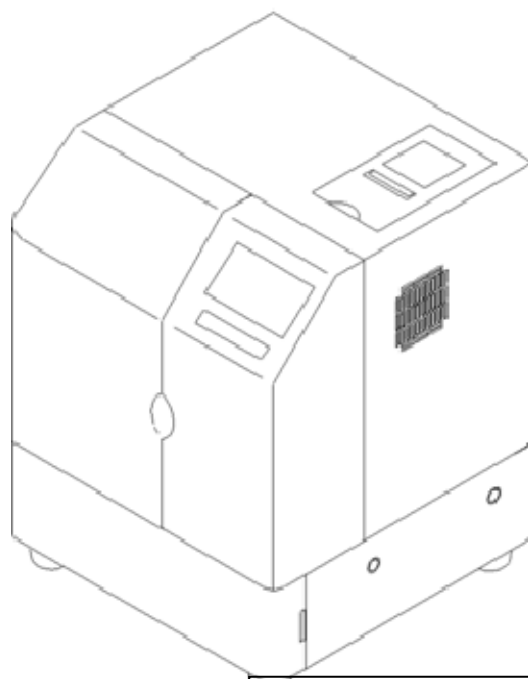

AUTOMATED ENZYME IMMUNOASSAY SYSTEM
AIA-360 (For in vitro diagnostic use)

1.3. System Outline

Fig. 1—2 Exterior View of AIA-360

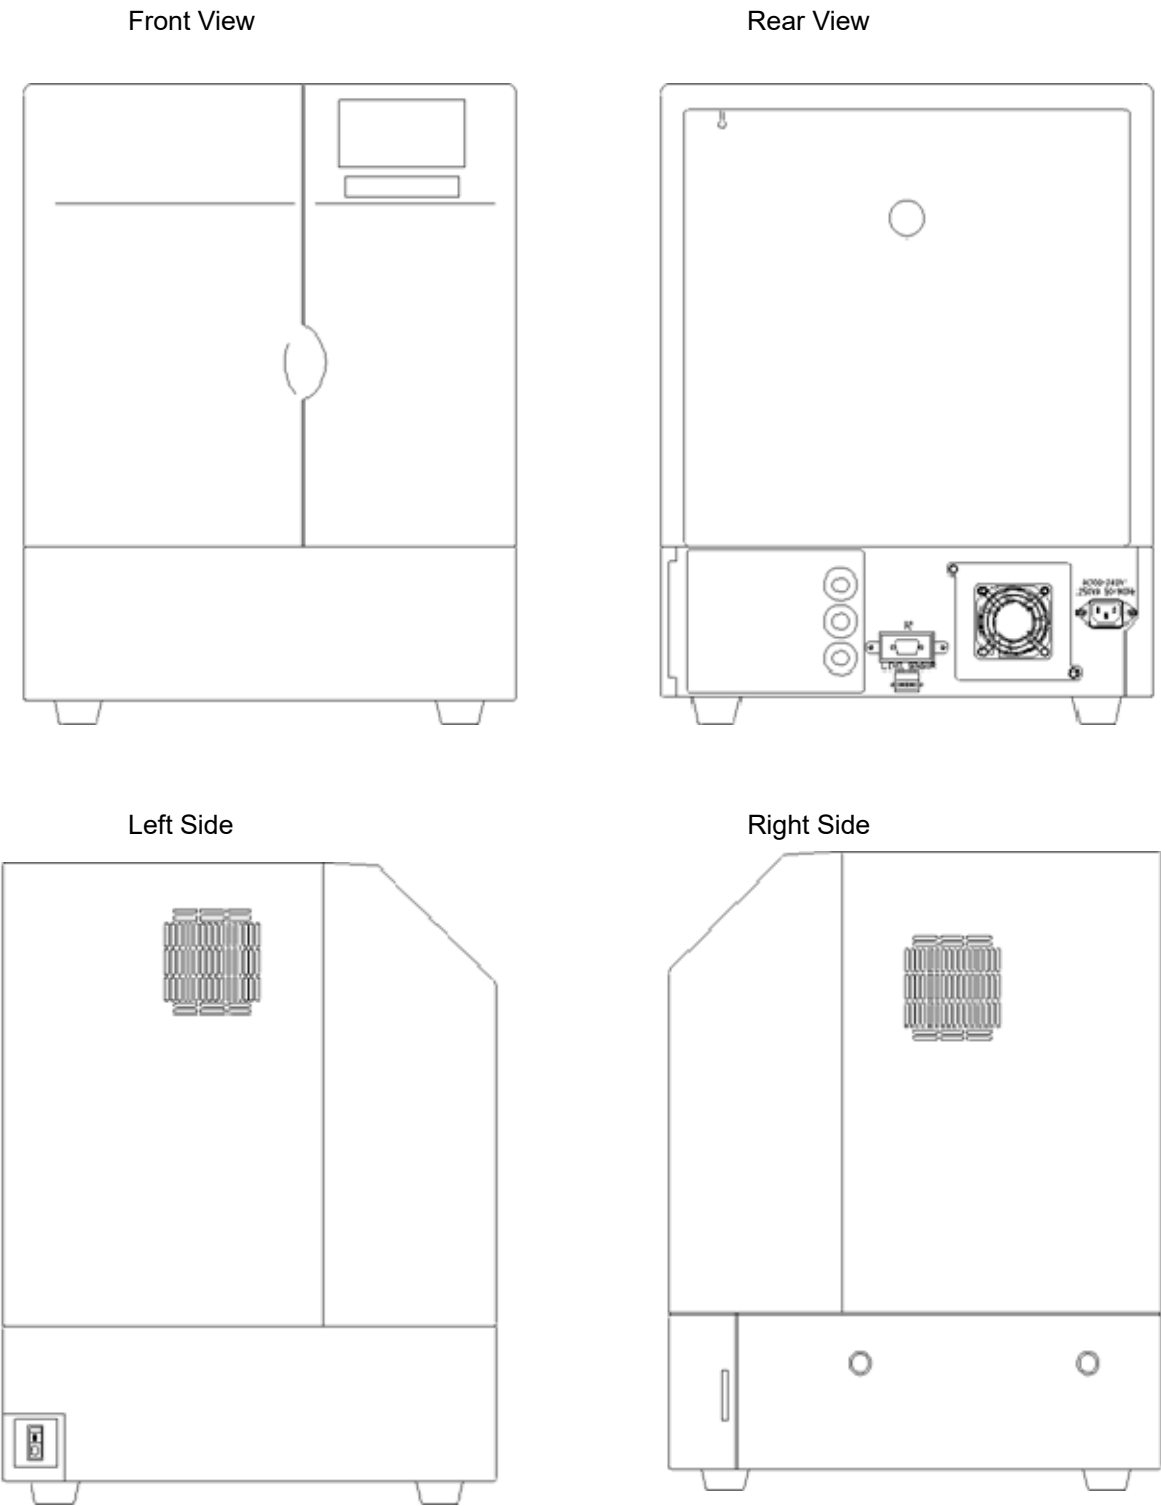

1.4. Specifications

Main Specifications

Assay principle	Fluorometric enzyme immunoassay (FEIA)
Processing method	Automated continuous random access
Processing capacity	Max. 36 tests / hr. (ST reagents)
In vitro diagnostic reagent (medical)	ST AIA-PACK Series
Sample volumes	10 to 100µl
Sample clog detection	Pressure detection
Measuring conditions	Reaction temperature: 37°C Antigen-antibody reaction time: 10 min.
Detection method	Fluorescent detection (top-to-top system)

Carousel

Reagent set count	Max. 25
Specimen set count	Max. 25
Sample containers	Test tubes(Φ13x 75, Φ 13x100, Φ16x75, Φ16x100) Combinable with dedicated sample cups
Specimen barcodes	CODE39, CODE128, ITF, NW-7 compatible (compliant with ASTM14466-92 and CLA guideline compliant barcodes) Min. element width (narrow): 0.191 (0.254 or over recommended)
External output	RS-232C
Power supply/consumption	100 to 240 V AC, 50/60 Hz, 250 VA
External Dimensions/Weight	Main unit: 400 (W) x 400 (D) x520 (H) mm, 29 kg

Operating Environment

Temperature	15°C to 30°C
Humidity	40 % to 80 % (no condensation)
Best	Average office level

Conformance Status

EMC standard	IEC61326-2-6: 2012
CISPR class and group categories	Class A, Group 1
FCC	Part15 Sub, Part B Class A
EMC standard	Class 1: IEC60825-1: 1994

1.5. Checking Packing Box Content

As a rule, Tosoh service personnel always set-up the system. You are requested to refrain from opening the packing box and attempting to install the system yourselves.

You are requested to confirm, in the presence of the Tosoh serviceperson, that all accessories in the following list are included with the system when it is unpacked.




The components of seven parts, diluent, wash solution and waste fluid bottles and caps, and the level sensor lead wire are different depending on the date of manufacture. Either set of parts “before change” or “after change” are provided with the instrument. For details of each item, see P.1-8 “before change” and P.1-9 “after change”. Note that the applicable seven parts cannot be used in combination with the parts “before change” and “after change”.

Packing List

Main Unit(AIA-360)

Accessories

- Power cable: 1
(Product no. 008272)




- Substrate bottle rubber stopper: 1
(Product no. 0021772)



- Bottle cap: 10



- Printer paper core: 1
(Product no. 0019510)



- Substrate holder: 1
screw and spacer: 2 pcs (each)
(Product no. 0021066)



- Bottle 30 ml: 2
(Product no. :0018619)




1.5. Checking Packing Box Content

- Bottle 100 ml with a cap: 1



- Bottle tray: 1
(Product no. 0021076)




- Smart media card: 1

Or



- USB stick: 1
(Including the initial parameters)



- Waste Box: 1
(Product no. :0019398)



- Tank filter: 2
(Product no. 0018585)



1.5. Checking Packing Box Content

[Composition of the seven parts before change (level sensor lead terminal: plug socket type)]

- Diluent bottle 500 ml
(DILUENT): 1
(Product no. :0021067)



- Wash solution bottle 1000 ml
(WASH): 1
(Product no. :0021068)



- Waste fluid bottle 1000 ml
(WASTE): 1
(Product no. :0021069)



- Diluent bottle cap: 1
(Product no. :0021103)



- Wash solution bottle cap: 1
(Product no. :0021140)



- Waste fluid bottle cap: 1
(Product no. :0021141)



- Level sensor lead: 1 set
(Product no. :0021138)



1.5. Checking Packing Box Content

[Composition of the seven parts after change (level sensor lead terminal: screw type)]

■ Diluent bottle 500 ml (DILUENT): 1 Optional Parts: Product no. 0024686 Part Name: DILUENT BOTTLE-2 WITH LABEL	
■ Wash solution bottle 1000 ml (WASH): 1 Optional Parts: Product no. 0024687 Part Name: WASHER BOTTLE-2 WITH LABEL	
■ Waste fluid bottle 1000 ml (WASTE): 1 Optional Parts: Product no. 0024687 Part Name: WASTE BOTTLE-2 WITH LABEL	
■ Diluent bottle cap: 1 Product no. 0024318. Part Name: DILUENT CAP ASSY-2	
■ Wash solution bottle cap: 1 Product no. 0024684. Part Name: WASH SOLUTION CAP ASSY-2	
■ Waste fluid bottle cap: 1 Product no. 0024685. Part Name: WASTE BOTTLE CAP-2	
■ Level sensor lead: 1 set Optional Parts: Product no. 0024317 Part Name: LEAD WIRE OF LEVEL SENSOR-2 With screws	

1.5. Checking Packing Box Content

Consumables

- Printer paper (thermal paper roll): 1
(Product no. :0019563)



- Sample cups: 100



- Detector Standardization test cups (STD cups): 1



Others

- Operator's manual CD: 1



- Inspection Certificate: 1



- Warranty: 1



The items listed above should be included in this package.
If any items are missing, immediately contact your local Tosoh representative.

Chapter 2: Installation

As a rule, installation and set-up of a newly delivered AIA-360 analyzer is performed by qualified Tosoh service personnel. You are asked to refrain from unpacking and installing the system yourselves.


2.1. Operating Environment

Make sure to install the system on a level table in an environment free from toxic fumes, dust, vibrations and exposure to direct sunlight.

Operate the AIA-360 within the range of conditions specified below.

Table 2-1 Operating Environment Conditions

Max. altitude:	2000 m
Temperature:	15 to 30°C
Humidity:	40 to 80%
Power supply/consumption:	100 to 240 V AC, 50/60 Hz, 250 VA
Overvoltage:	Category II
Contamination level:	2
Dust level:	equivalent to average office environment



Make sure to operate the AIA-360 within the range of conditions specified in the table above in an environment free of moisture from condensation.

2.2. Environment of transportation and storage


Transport and store the instrument under the following conditions if it is moved to another place and re-installed.

Temperature:	5 to 50°C
Humidity:	80% or less
Dust level:	Keep dry, store indoors

2.3. Installation Environment

Avoid installing the AIA-360 in locations subject to the following types of conditions


- Sharp fluctuations in power supply voltage

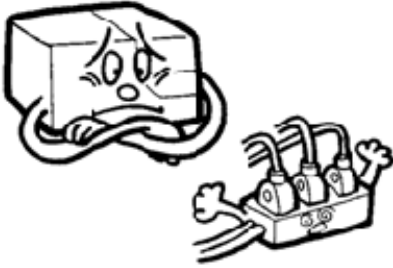

- Sharp fluctuations in temperature




- Powerful air currents

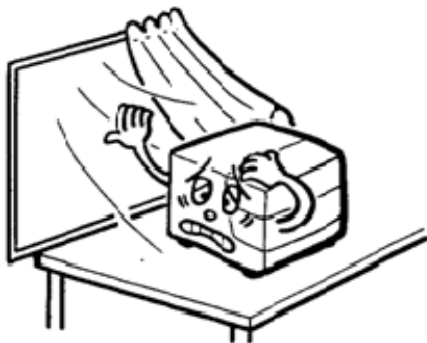

- Excessive dust



- Excessive vibrations

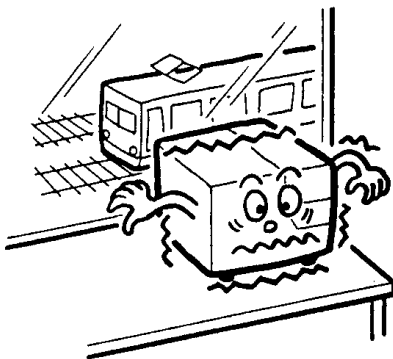


- Unstable foundations



2.3 Installation Environment

- Locations with high humidity (> 80 %)
- Locations near water sources, such as a sink

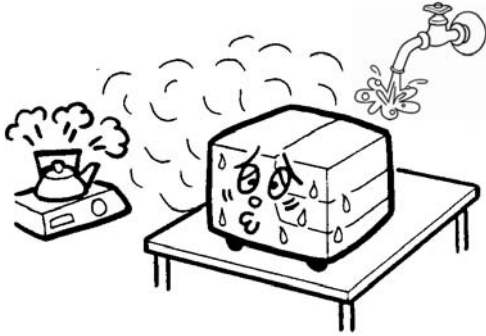


- Open flames



- Narrow spaces with poor ventilation



- Strong electromagnetic fields and high frequencies

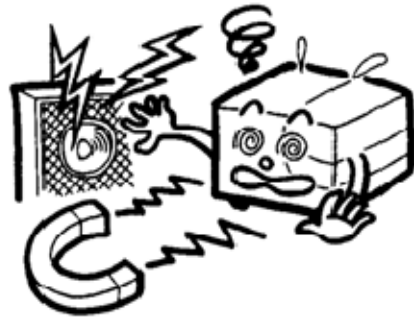

2.4. Space Required for Installation


The dimensions of the AIA-360 are 400 mm (W) x 400 mm (D) x 520 mm (H). In addition to these dimensions, the AIA-360 requires extra space on the right side for the external attachment of the bottle tray for the diluent, wash solution and waste fluid bottles.

For ventilation purposes an electric fan is installed on the rear of the unit. Provide an extra margin of at least 150 mm at the back to allow the fan to function properly.

Also allow a margin of at least 250 mm on the left side to open the carousel door when loading samples and reagent cups.

The standard system weight of 29 kg increases to about 35 kg when the reagents are loaded. Make sure that the base on which the AIA-360 is installed is sufficiently strong to withstand this weight without vibrating.


Fig. 2-1 Space Required for Installation

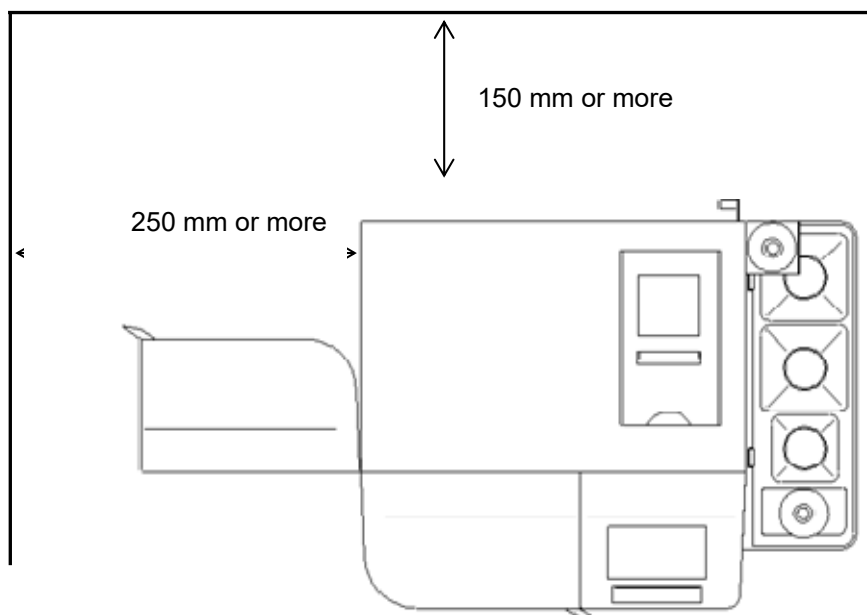

2.5. Installation Procedure

Connecting Tubing

Fig. 2-2 Port Branching Assembly

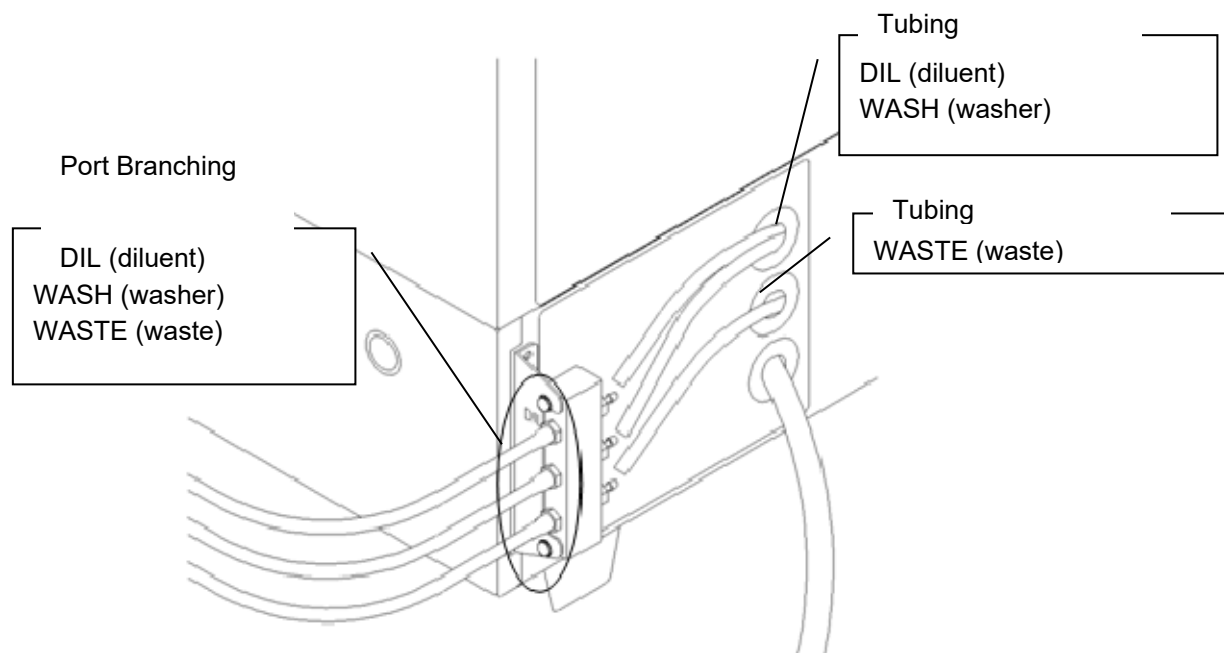

- (1) Connect the tubes extending from the rear of the AIA-360 to the port branching assembly as shown below.

Diluent (DIL) tube	→ Port branch DIL
Wash solution (WASH) tube	→ Port branch WASH
Waste fluid (WASTE) tube	→ Port branch WASTE




Identification seals are attached to each tube. Use these to ensure tubes are connected to the correct port. Errors will result in incorrect assay results.

- (2) Connect the tubes linked to the port branching assembly to the caps on each of the bottles.

2.5. Installation Procedures

- (3) Tighten the bottle caps and arrange them in the order shown in Fig. 2-3, starting from the front with the diluent bottle, wash solution bottle, and waste fluid bottle.

Fig. 2-3 Bottle Installation Order

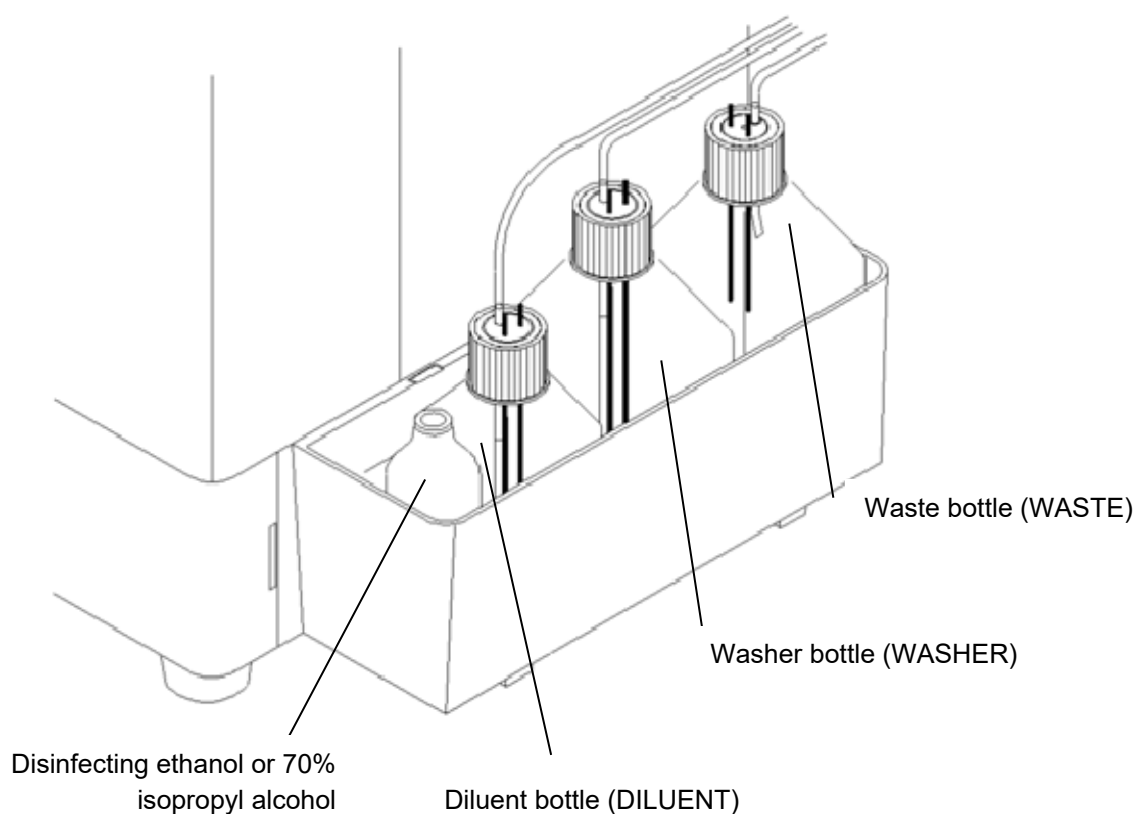


The wash solution and waste fluid bottles are identical in shape, so be sure to check the identification seals to prevent any mix-ups. Mistakes will result in incorrect assay results.

2.5. Installation Procedures

Connecting Level Sensor Lead Wire (Before Change)

Fig. 2-4-1 Level Sensor Lead Wire (Plug Socket Type)

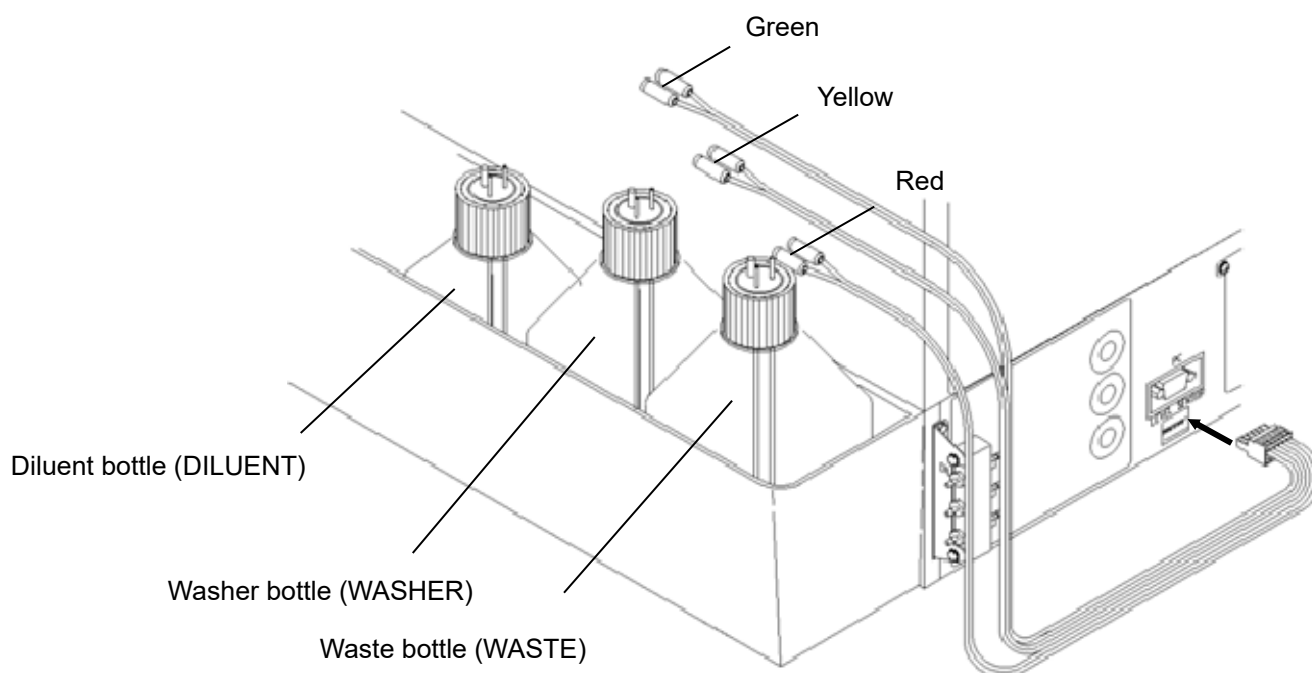

- (1) Connect the connector at the end of the level sensor lead wire in the direction of the arrow shown in the figure above.
- (2) Use the colour coding on the terminals of the level sensor lead wire to ensure that they are correctly connected to the electrodes for each bottle.

Waste fluid bottle (WASTE)	→ red
Wash solution bottle (WASHER)	→ yellow
Diluent bottle (DILUENT)	→ green




Make sure that level sensor lead wire connectors are correctly matched. Incorrectly connecting the lead wire will result in failure to issue warnings when the diluent and washer levels are low or when the waste tank is full.

2.5. Installation Procedures

Connecting Level Sensor Lead Wire 2 (After Change)

Fig. 2-4-2 Level Sensor Lead Wire-2 (Screw Type)

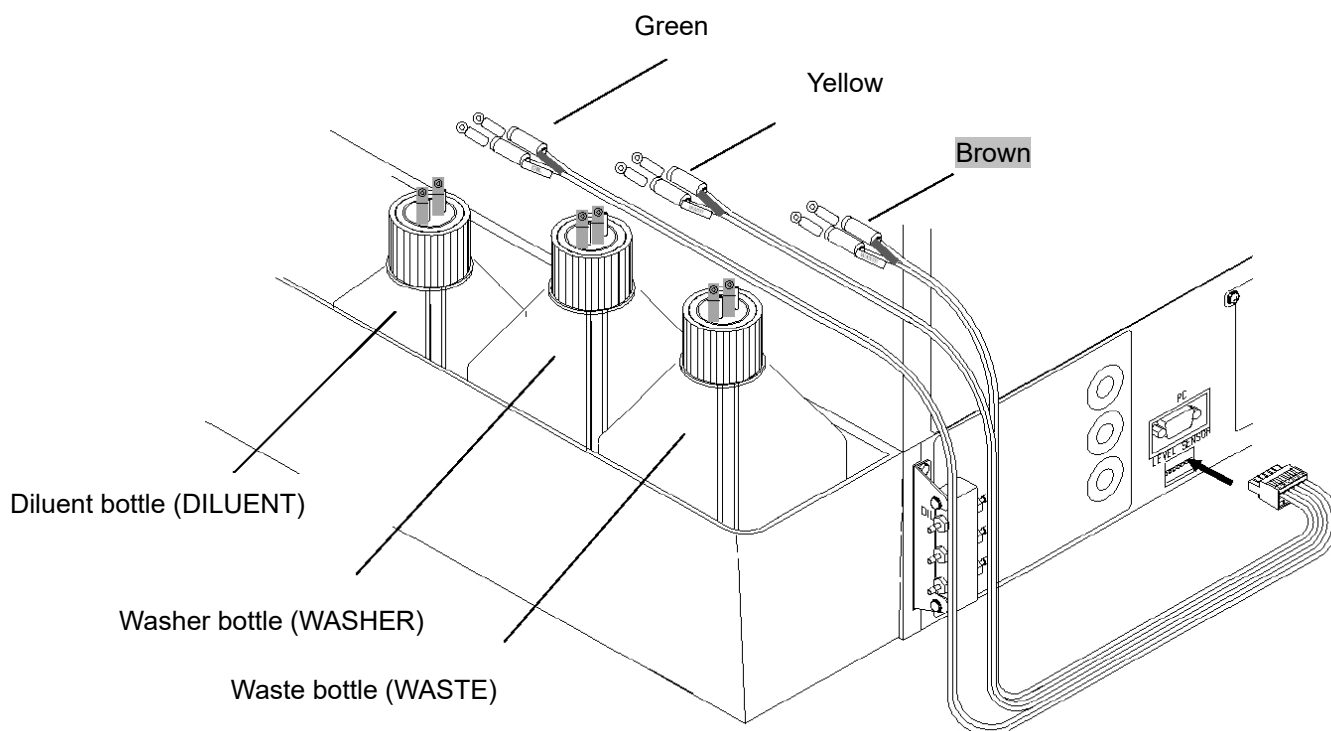

- (1) Connect the connector at the end of the level sensor lead wire 2 in the direction of the arrow shown in the figure above.
- (2) Use the colour coding and identification names on the terminals of the level sensor lead wire 2 to ensure that they are connected properly and firmly to the electrodes for each bottle 2 using the provided screws, and then cover the terminals with the rubber protection caps.

Waste fluid bottle (WASTE)	→ brown
Wash solution bottle (WASHER)	→ yellow
Diluent bottle (DILUENT)	→ green




Make sure that level sensor lead wire 2 connectors are correctly matched. Incorrectly connecting the lead wire 2 will result in failure to issue warnings when the diluent and washer levels are low or when the waste tank is full.

2.5. Installation Procedures

Installing Printer Paper


- (1) Open the printer cover (top) by lifting upward.

Fig. 2-5 Printer

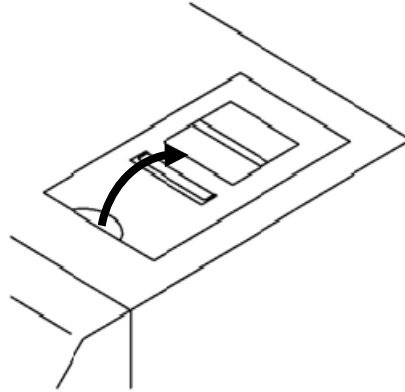

- (2) Pull the paper clamp lever to the full forward position and remove the paper core shaft by pulling upward.
- (3) Insert the core shaft into the paper roll and install it in the printer so it faces the correct direction.


Fig. 2-6 Installing Printer Paper

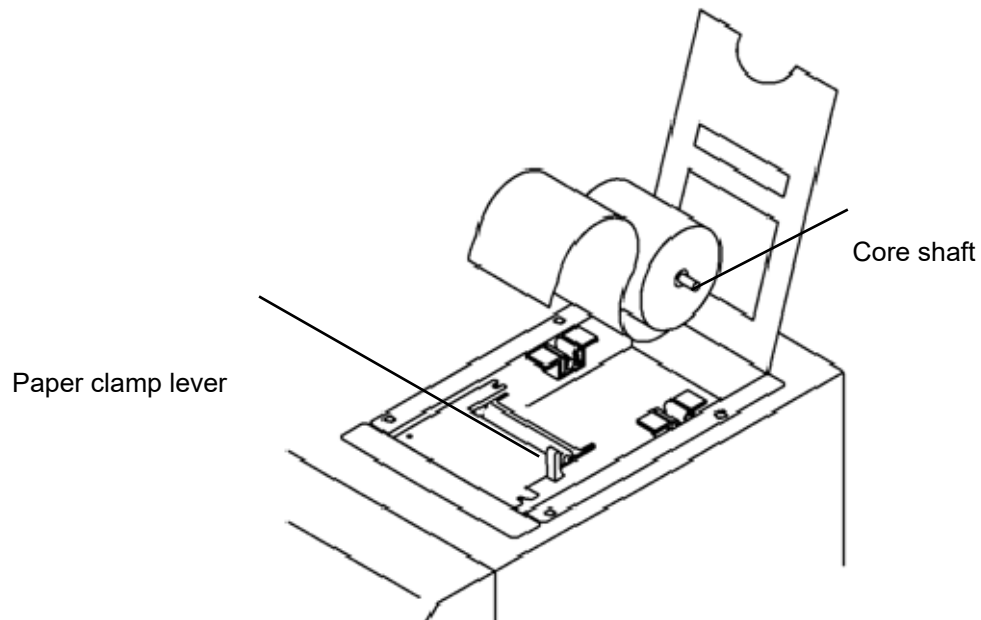

2.5. Installation Procedures

- (4) Return the paper clamp lever to its full back position and insert the tip of the paper into the printer mechanism.

Fig. 2-7 Installing Printer Paper

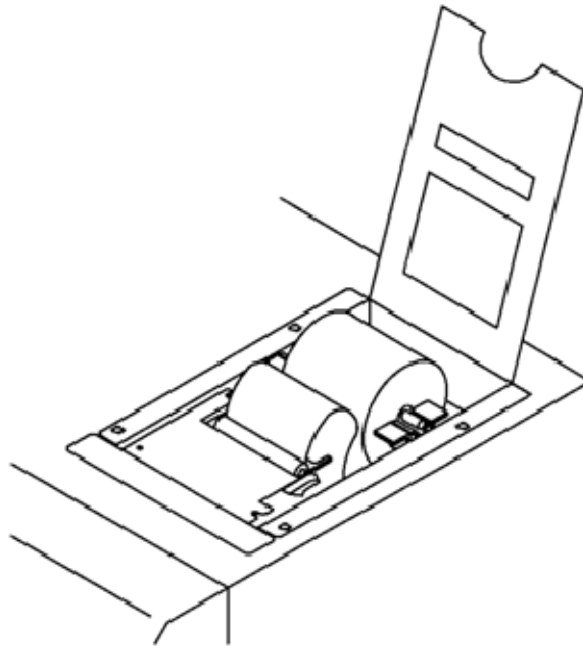

Note that the lever has two settings, so make sure to set to the full back position.

- (5) Close the printer cover (top), while remembering to pass the end of the printer paper through the cover's paper opening.




If paper is not positioned correctly, pull the paper clamp lever to the forward position and adjust, then return lever to full back position.

2.5. Installation Procedures


Installing Enzyme Substrate Fluid

Fig. 2-8 Attachment of the Substrate Solution Holder (1)

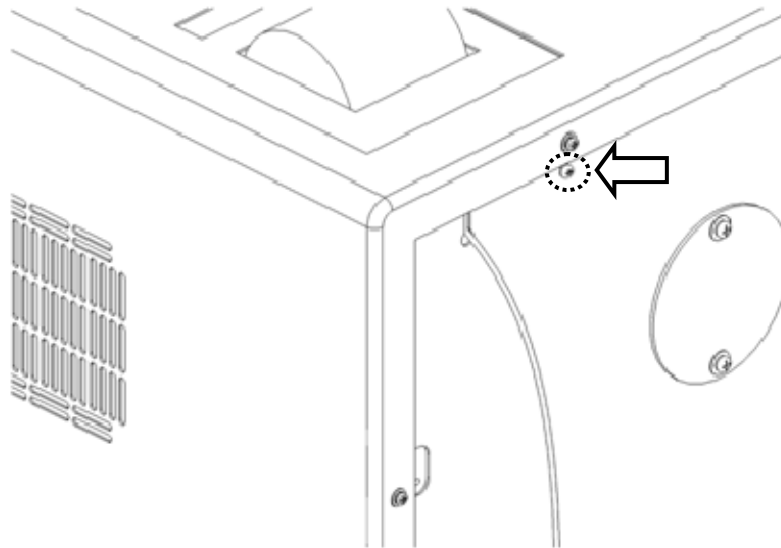

(1) Remove the screw shown in Fig. 2-8 (The removed screw will be of no use).

Fig. 2-9 Attachment of the Substrate Solution Holder (2)

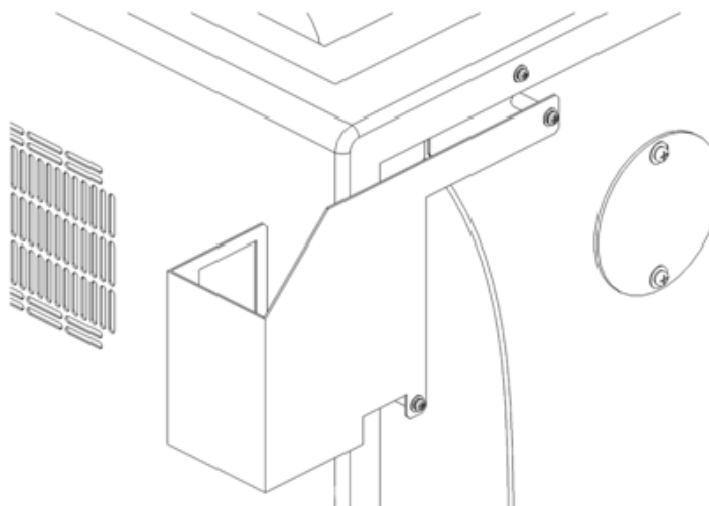


(2) Using the screws and spacers included in the accessory kit, attach the substrate holder as shown in Fig. 2-9.



The substrate solution tube passes through and beneath the holder.

2.5. Installation Procedures

Fig. 2-10 Substrate Solution Holder and Enzyme Substrate Bottle

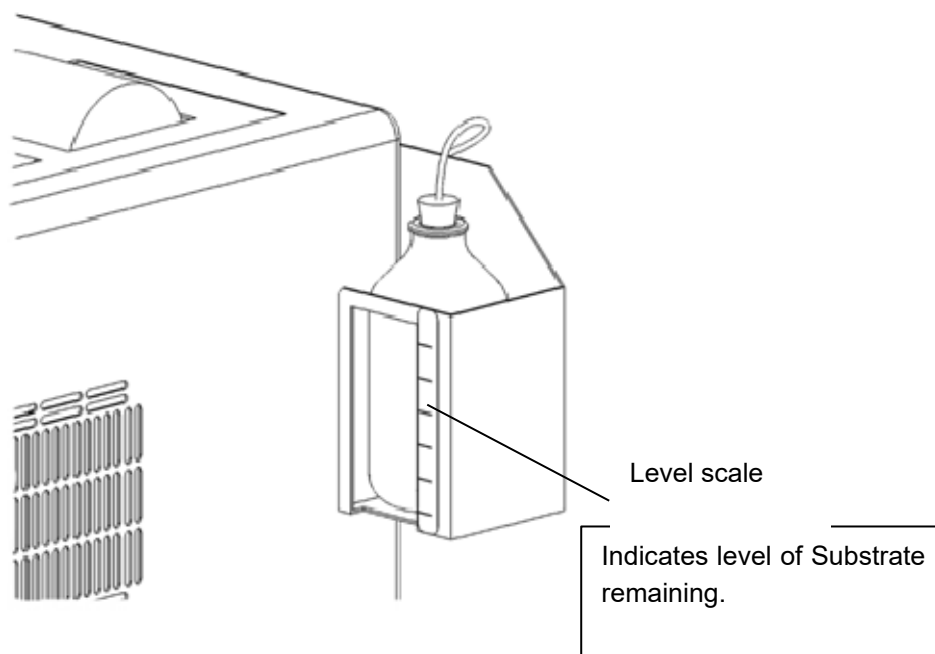

- (3) Set the substrate bottle on the holder (See Fig. 2-10).
- (4) Put the substrate solution tube deeply into the substrate bottle and plug the bottle with the rubber cap.



Put the tube into the bottle until the tube end touches to the bottom of the bottle.

2.6. Power Supply

(1) Confirm the following system power supply specifications.


Power specifications: 100/120V AC and 220/230V AC ± 10 V
250 VA
50/60 Hz



- Connect the AIA-360 using the accessory power cable grounded to the power supply socket (10 A).
- Avoid connecting the AIA-360 to the same power socket as other equipment, such as refrigerators and compressors that consume large volumes of power.
- Use only a power supply line equipped with circuit protector.

(2) After confirming that the power supply switch located on the left rear of the system is set to the OFF position, insert the power supply cable into the socket.

Fig. 2-9 Power Supply Socket

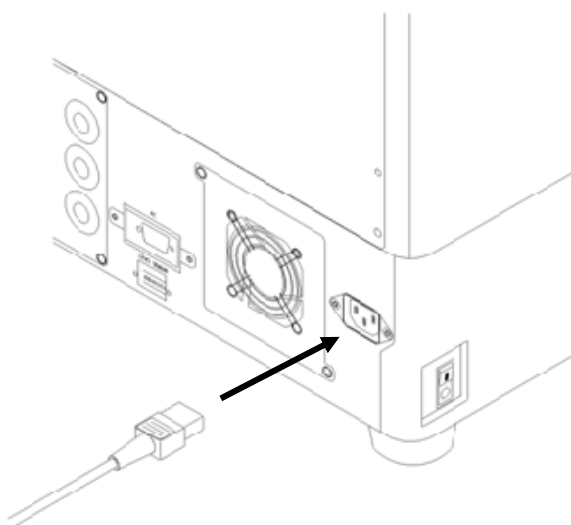


Point

Note that the position marked "O" is OFF and the position marked "I" is ON. Wait at least 10 seconds before turning on the instrument again after having turned it off.

Chapter 3: Name of Parts and Functions on Main Unit

The AIA-360 is comprised of the modules illustrated below.

Fig. 3-1 Overview of Main Unit

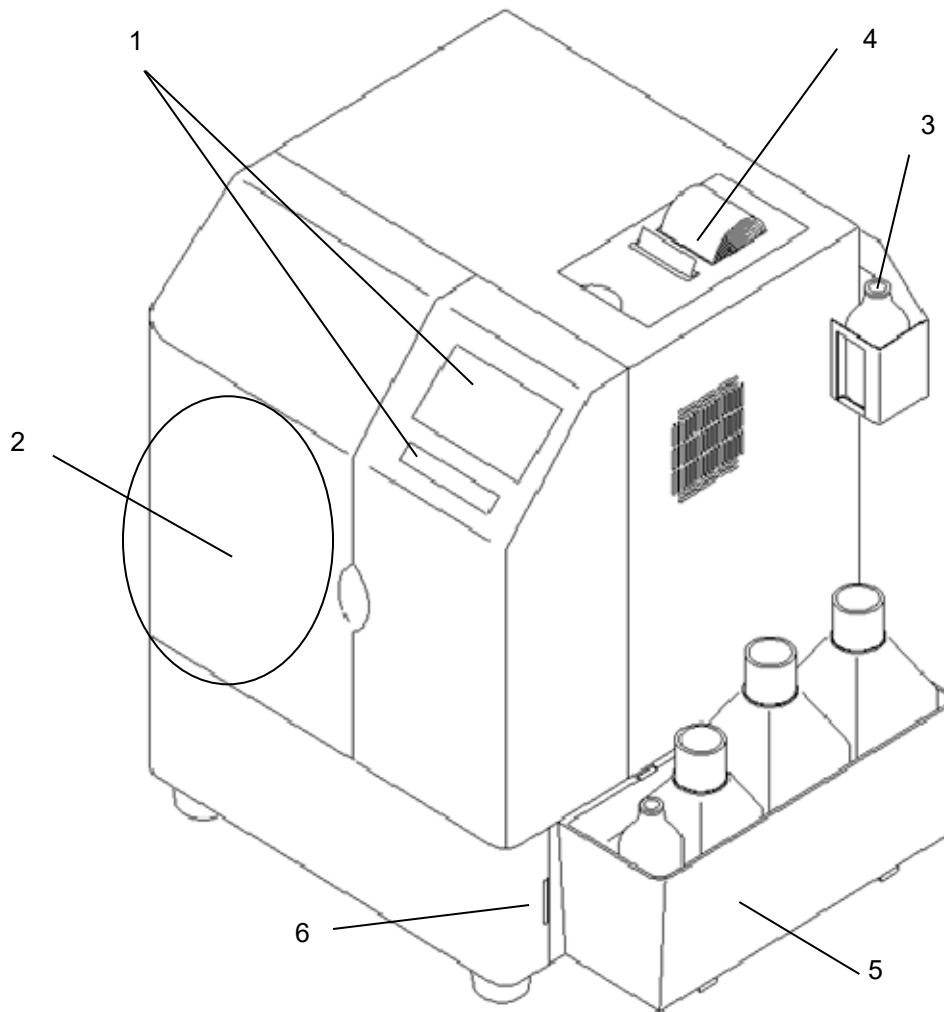


1. Display and operation panel
2. Carousel (located inside door)
3. Substrate compartment
4. Printer unit
5. Bottle tray
6. External recording media slot

3.1. Display and Operation Panel

A LCD touch-panel equipped with sheet keys serves as both the display and key entry device for the AIA-360.

The LCD display is located on the front right side (when facing front) of the main unit. The display shows the operating status of the current system and the assay results.

Fig. 3-2 Display and Sheet Keys (Sample)

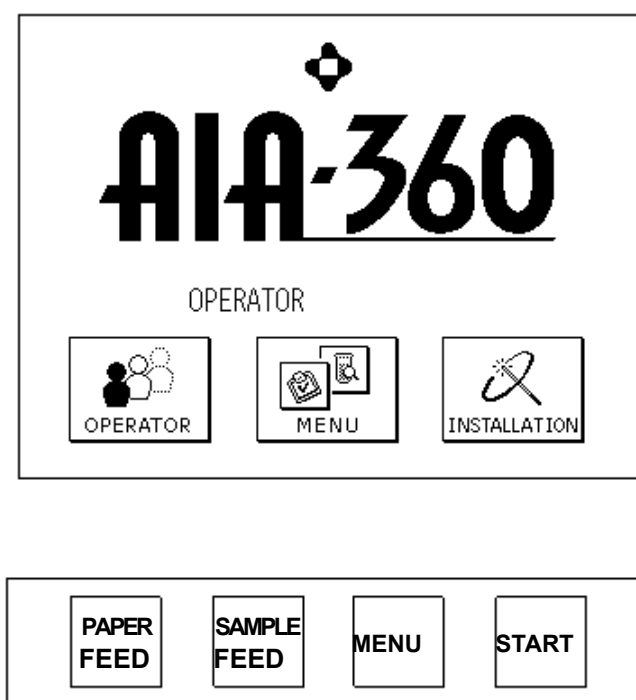

Paper Feed Key

Used to feed printer paper.

Sample Feed Key

Moves the sample carousel forward by 1 cup.

Menu Key

Displays the menu screen.

Start Key

Starts the assay operation.




Do not press the START key for a long time.

Depressing the START key for a long time (about two seconds or longer) sends an abort request for an emergency stop, and prints a warning message.

3.2. Carousel


The main carousel is the unit that serves as both the reagent cup holder and the sample holder. The carousel is designed to rotate the specimen and reagent cups. Seven reagent cup holder slots and seven sample holder slots are visible when the carousel door is opened.

Fig. 3-3 View with Carousel Door Open

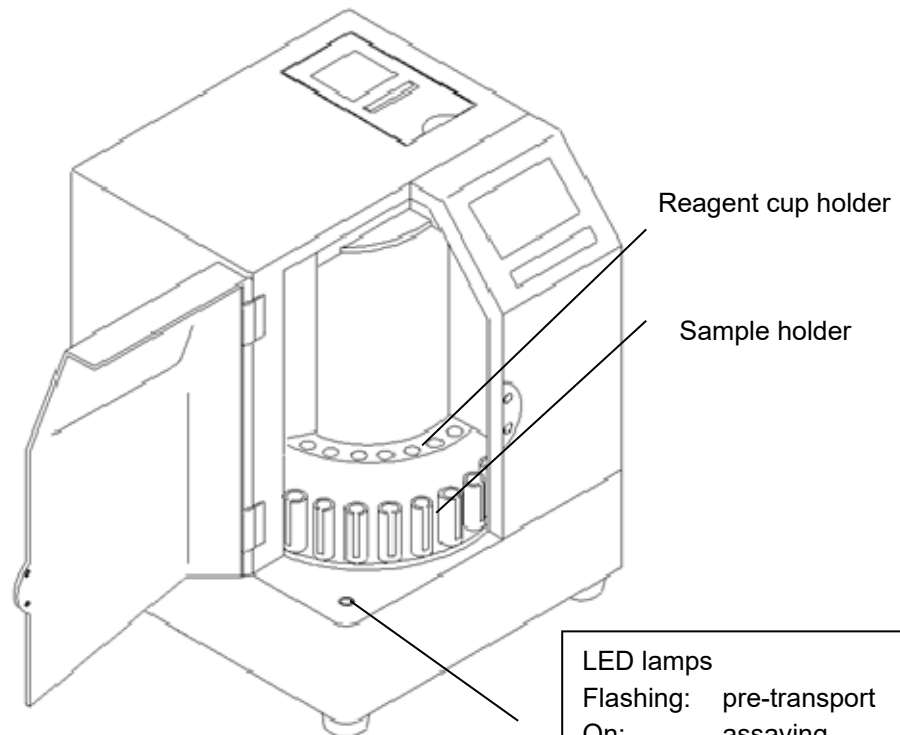

Point

- When the **SAMPLE FEED** key is pressed for two seconds or longer, the carousel rotates automatically and returns to its home position.
- To stop the carousel from automatically rotating, press the **SAMPLE FEED** key once again.



Be careful not to get your fingers caught when the carousel moves.

3.3. Substrate Compartment

This compartment is used for the enzyme substrate bottle and the 70% ethanol or 70% isopropyl alcohol solution bottle.

3.4. Printer Unit

The printer is designed to the print assay results, error information and system parameters onto a roll of thermal printer paper. Depending on the font selected, the printer can print the assay results for up to 2000 test cups on one roll of paper.

3.5. Bottle Tray


Note that the diluent, wash solution and waste fluid bottles and the 70% ethanol or 70% isopropyl alcohol solution bottle are stored outside rather than inside the main unit.

3.6. External Recording Media Slot

The system program is updated using external recording media.

Chapter 4: Preparing System for Assay Operations

4.0. Introduction

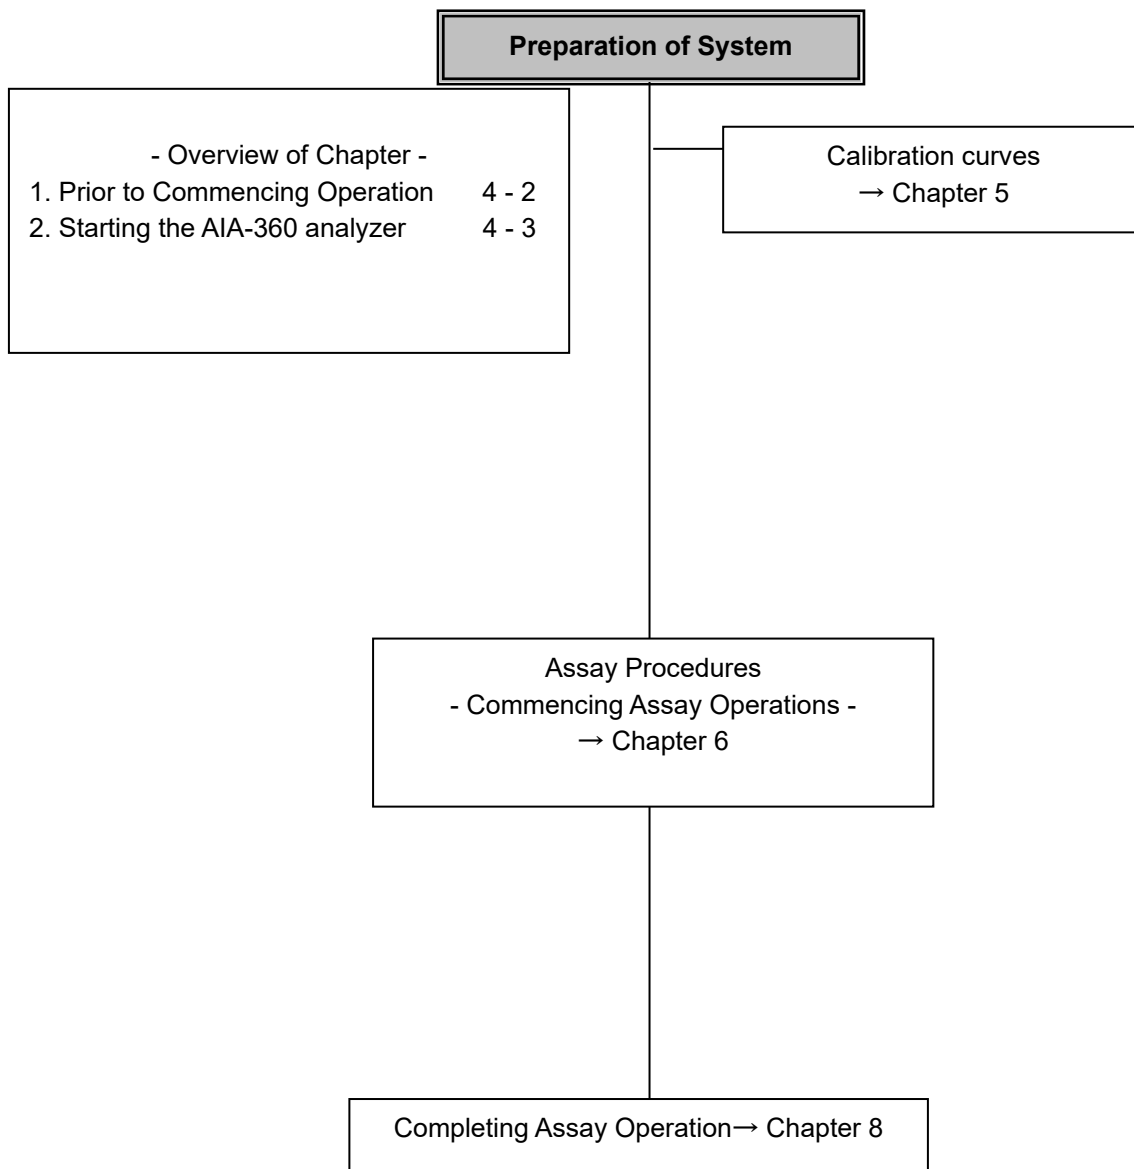

4.1. Prior to Commencing Operation

The following items are required for performing assay operations.

- Reagent cup
- Enzyme substrate solution
- Detector standardization test cup (STD cup)
- Diluent and wash solution
- 70% Ethanol or 70% isopropyl alcohol
- Samples (patient specimens and calibrators)



Make sure to properly mix the substrate, diluent and wash solutions in accordance with the instructions provided in the manual.

The following two types of samples are used for assay operations in the AIA-360.

- (1) Patient specimens
- (2) Calibrators (standards)

(1) Assaying Patient Specimens

Prepare the specimens and reagent cups. Dispense the required volume of specimen into the sample cup or primary tube. The required specimen volume is defined as the sum of all dispensed analyte volumes, plus the dead volume.

Dead volume: 100 µl for sample cups.
approximately 500 µl for the straight type Φ 11 mm primary tubes but varies depending on tube bore and shape.



Up to four analytes can be assayed from a single specimen. However, the specimen must be divided into two portions whenever assaying five or more analytes from a single specimen.



Applicable specimen type for the AIA-360 is indicated on the insert sheet provided with reagents for each analyte. Users are asked to avoid assaying the following types of specimens, as they can affect system operation.

- Specimens that have a tendency to clot during the assay process.
- Specimens containing solid particles that tend to form occlusions during dispense operations.

(2) Generating Calibration Curves

Prepare calibrator and reagent cups. Measuring calibrators is necessary when generating calibration curves. Begin by compiling an appropriate calibration program, then prepare calibrators and reagent cups and perform measuring operations accordingly.

4.2. System Start-up

4.2.0. System Start-up


BEFORE TURNING ON POWER

Open the operation cover on the main unit and confirm there is nothing blocking the movement of the carousel.

- (1) Next, go to the system power switch located on bottom left rear of the main unit and switch it to ON.

Fig. 4-1 Power switch

Power switch

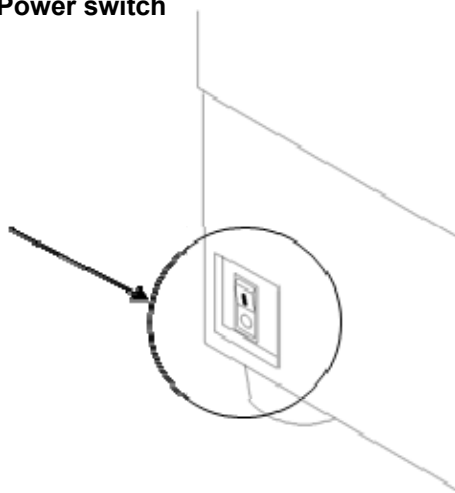



Point

Note that the position marked “O” is OFF and the position marked “I” is ON.

4.2.0. System Start-up

- (2) When system power is turned on, the Now Loading Screen, the Start Program Screen and the OPENING Screen of the AIA-360 are displayed in this order on the display.

* A display type exists in which the Now Loading Screen and the Start Program Screen are not displayed.

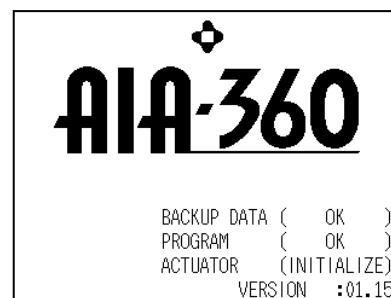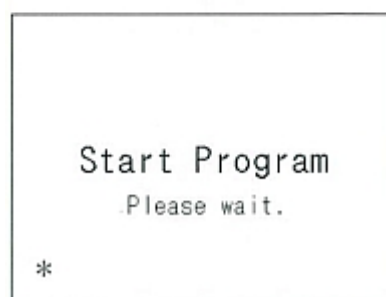

Pressing  displays the factory default system installation procedures.

As a rule, installation of a newly delivered AIA-360 is performed by qualified Tosoh service personnel. Customers are asked to refrain from unpacking and installing the system themselves.



<OPENING Screen>

4.2. System Start-up

4.2.1. Confirming/Selecting Operator Name

- (1) Confirm the current operator name displayed in the OPENING screen.

Point

The operator name is also printed on the printouts.

- (2) If the correct operator name is displayed, simply press the  icon.
(Proceed to section “2.2 Confirming Enzyme Substrate Solution Level.”)

- (3) To change the operator name, simply press the




icon. Use   to move the cursor to

the desired operator name then press the



icon to select.

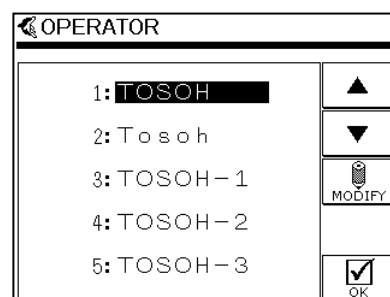


<OPERATOR Screen>

Registering New Operator Name

The AIA-360 analyzer allows registration of up to 5 operators, which are retained even when the power is turned off.

- <1> Press the  icon.

This displays the OPERATOR Screen.

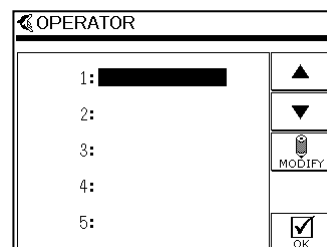


<OPERATOR Screen>

- <2> Use   to move the cursor to the new operator number to be registered.

Then press the  icon.

This displays the KEYBOARD INPUT screen.

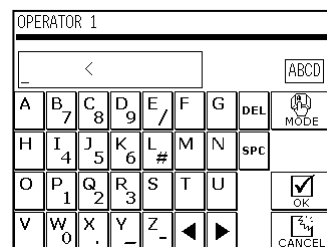

<KEYBOARD INPUT Screen>

Point

Pressing the  icon displays the following content.



Alphabet (uppercase)



Alphabet (lower case)



Numerals

4.2. System Start-up

<3> Register operator name (using up to eight characters).

<4> Press the  icon after entering the name and return to the Operator Screen.

Changing/Deleting Operator Names

<1> Press the  icon to display Operator Screen.


<2> Use   to move cursor to operator number

to be deleted and press the  icon.

This displays the KEYBOARD INPUT Screen.


<3> Press the  to delete when changing or deleting the operator name.

<4> When name change is successful, press the  icon.

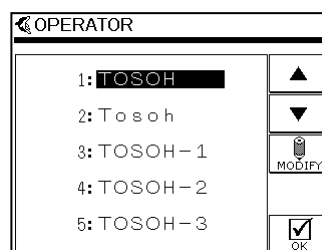

The OPERATOR screen displays a list of operators. The first operator, '1: TOSOH', is highlighted. To the right of the list are three buttons: an up arrow, a down arrow, and a 'MODIFY' button. At the bottom right is an 'OK' button.

<OPERATOR Screen>

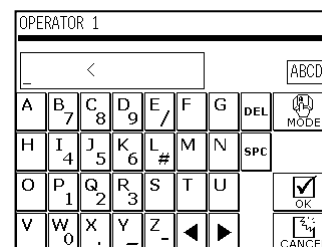


The KEYBOARD INPUT screen shows 'OPERATOR 1' at the top. Below it is a text input field with a cursor. To the right of the field is a 'MODE' button. Below the input field is a grid of buttons for letters A-Z, numbers 0-9, and symbols like DEL, SPC, and arrows. At the bottom right are 'OK' and 'CANCEL' buttons.

<KEYBOARD INPUT Screen>

4.2. System Start-up

4.2.2. Confirming Enzyme Substrate Solution Level

- (1) The SUBSTRATE Screen is displayed.
- (2) Enter the enzyme substrate solution level indicated on the solution level scale.
- (3) Next, press the  icon.

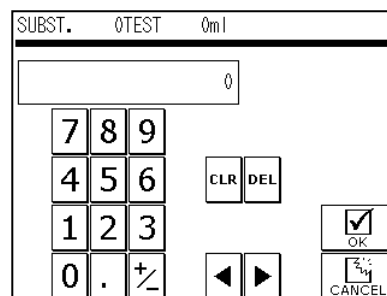

<SUBSTRATE INPUT Screen>



- **Note that the correct enzyme substrate solution level must always be entered.**
- **Failure to do so will result in DAILY CHECK errors.**
- **Also be sure to enter the new substrate level in the SUBSTRATE screen whenever installing a new enzyme substrate solution.**

Point


The current level of enzyme substrate solution can be checked by going to the **START UP** screen and pressing  or by going to the **ASSAY MONITOR** screen and pressing the  icon.

This displays the **SUBSTRATE** screen, which indicates the current level of solution and number of assay tests possible with this solution.

4.2. System Start-up


4.2.3. DAILY CHECK

(1) The MENU screen is displayed.

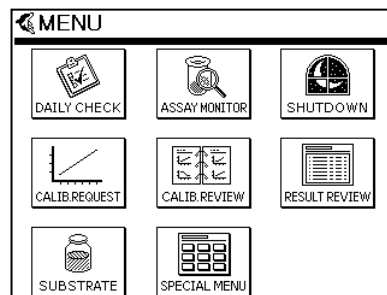

<MENU Screen>

(2) Press the  icon in the MENU screen to display the DAILY START CHECK screen. Then check the following items.

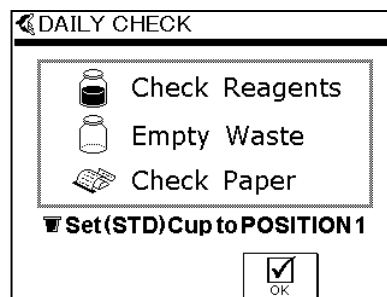

<DAILY START CHECK Screen>

- Check Reagents
Make sure there is sufficient WASHER (Wash Solution) and DILUENT (diluent).
- Empty Waste
Discard waste fluid and empty the waste tank (WASTE).
- Check Paper
Check to see that there is sufficient printer paper.

(3) In accordance with the “Set (STD)Cup to POSITION 1” instructions, place one detector standardization test cup (STD cup) in position No. 1 in the Reagent Cup table.

(4) Then press the  icon.

After the  icon is pressed, the following errors may occur.

- Error No.3023 PM DUE: Periodic Maintenance due.
- Error No.3024 PM REQUIRED: Periodic Maintenance is required.

If these errors occur, please contact the local Service department for maintenance.

4.2. System Start-up

- (5) When DAILY CHECK screen appears, press the **START** key.
Fluid supply lines automatically fill and a substrate background measurement is performed (enzyme substrate fluorescent intensity check).




<DAILY CHECK Screen>




The **DAILY CHECK** requires approximately seven minutes.

[SCREENS THAT APPEAR DURING THE DAILY CHECK]


Confirmation of initialization sequence

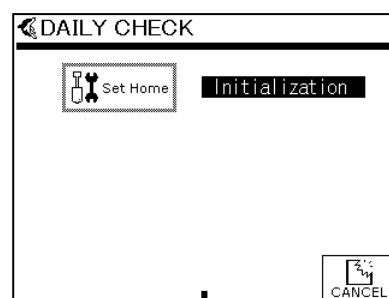

Priming of diluent

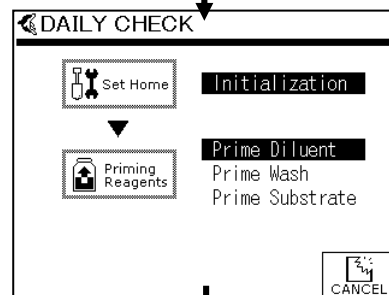


Priming of wash solution

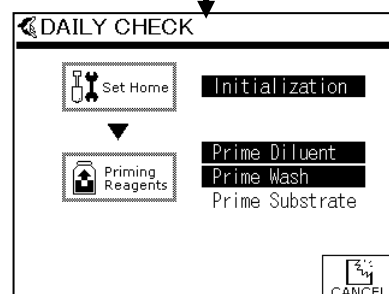


When errors occur during priming of diluent or wash solution, check bottle level and confirm the tube reaches down to the fluid.

4.2. System Start-up


Priming of substrate

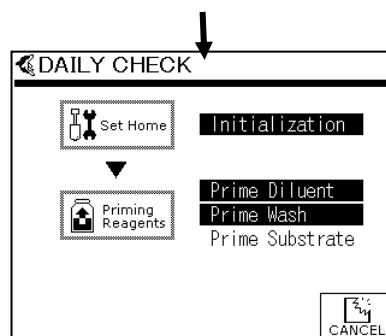

Measuring substrate background

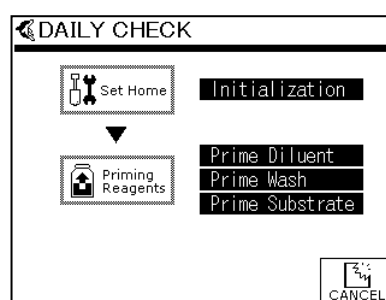

When errors occur during substrate background measurement, check substrate level and whether substrate has been replaced with 70% ethanol or 70% isopropyl alcohol.

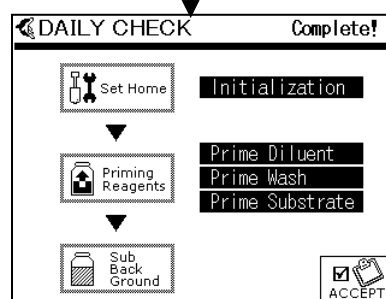


In the Event of Errors

An error message is displayed at the top left of the DAILY CHECK screen whenever an item deviates from the normal operating range.



Press the **CANCEL** icon to return to the START UP screen.

Redo the DAILY CHECK once corrective measures have been taken.

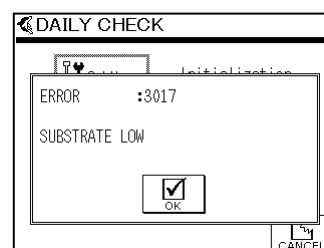

<ERROR Screen (Example)>

4.2. System Start-up

- (6) Sample lines are initialized and the results output to the printer when the substrate background measurement operation is complete.

Fig. 4-2 Sample Printout

```

***SUBSTRATE BACKGROUND ***
OP:          10/07/01 13:28

Date       : 10/07/01 13:28
SubstrateReplacement:OK
4MU Background :OK
50
LampIntensity Level :OK
BG Smp       :990
BG Ref       :1352
Subst Smp    :2113
Subst Ref    :25236
***END***
  
```

Arrows point from the following lines to numbers 1 through 4 on the right:

- SubstrateReplacement:OK → 1
- 4MU Background :OK → 2
- 50 → 4
- LampIntensity Level :OK → 3

- (1) Indicates whether the enzyme substrates solution priming operation was successful by 'OK' or 'ERR'. When the detector lamp intensity decreases, an 'ERR' appears too.

OK: When successful

ERR: When unsuccessful or the detector lamp intensity decreases.

→ Check substrate level and perform DAILY CHECK again.

When 'ERR' appears again, please contact your Tosoh local representative.

- (2) Performs fluorescent intensity (background intensity) measurement of enzyme substrate solution to check for possible problems. This measurement result is reported by 'OK' or 'HB' with measurement value in nmol/L.

OK: When lower than 1500 nmol/L (No problem)

HB: When equal to or higher than 1500 nmol/L (Background was too high)

→ Replace the enzyme substrate and perform DAILY CHECK again.

- (3) Indicates intensity of Detector lamp by 'OK' or 'LL'.

OK: If sufficient

LL: If insufficient

→ Please contact your Tosoh local representative.

- (4) Measurement value

- (7) Press the  icon.

4.2. System Start-up

When Starting Assay Before Daily Check is Completed Successfully

In any of the following cases, a warning message will appear indicating that the daily check has not been completed successfully.

- When starting specimen assay or calibration after turning on the instrument, without performing daily check



- When starting specimen assay or calibration after shutting down the instrument, without performing daily check
- When starting specimen assay or calibration after daily check has been terminated abnormally




Pressing  cancels the start of specimen assay and calibration. Perform daily check if necessary.



The warning message appears only once. Regardless of whether daily check has been performed or not, the warning message will not appear at the next assay start.

Chapter 5: Calibration

5.0. Introduction

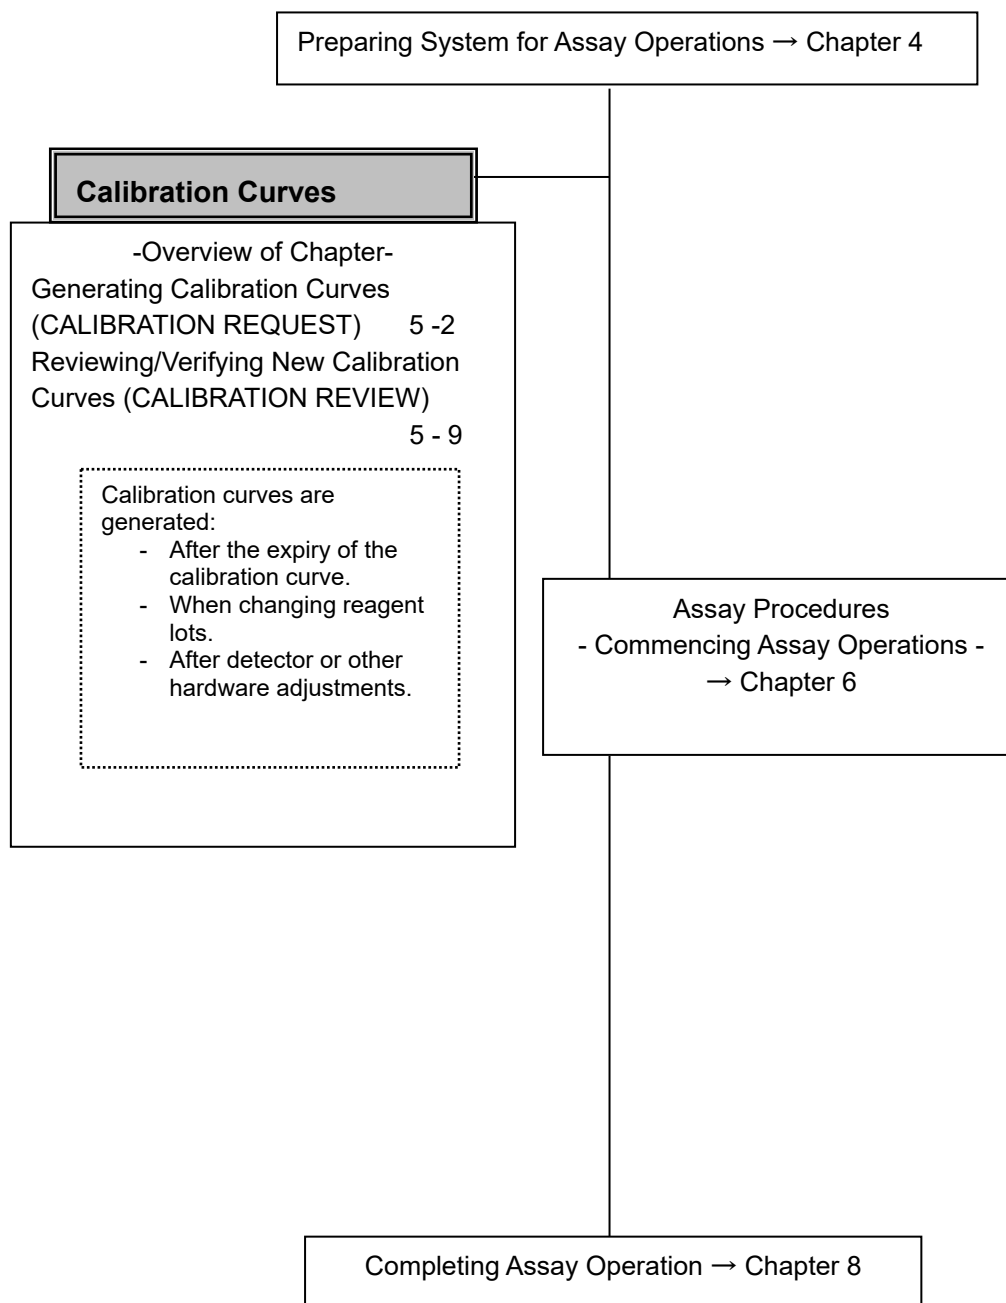

5.1. Generating Calibration Curves

5.1.1. Calibration Requests

Procedures for generating calibration requests are described in the following sections.



Note that calibration curves cannot be generated during assay operations. Sample measurement cannot be performed during calibration.


Procedures

- (1) Press the **MENU** key to display the MENU Screen.




<MENU Screen>

- (2) Press  to display the CALIB REQUEST screen.

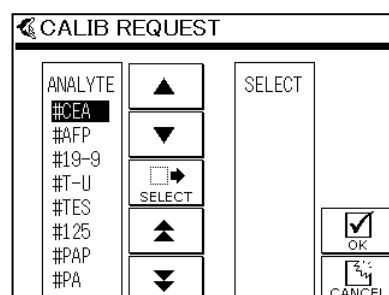

<CALIB REQUEST Screen>

- (3) Press   to move the cursor to desired item and press  to select.

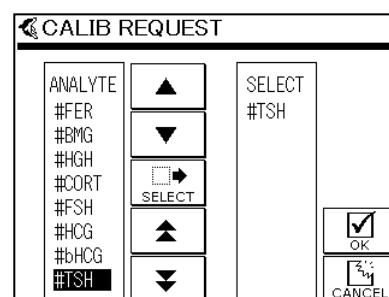

Point

Pressing   moves the display to the next page.



Note that the number of analytes that can be calibrated is four for a two-point calibration, one for a 6-point calibration and one for a combined two-point and six-point calibration

5.1. Generating Calibration Curves

(4) Pressing  displays the CALIB REQUEST (Conc. Set) screen.

(5) Confirm that the concentration matches the concentration listed on the calibrator label.

ANALYTE	CAL	CONC	UNIT
#TSH	CAL1	0.00000	uIU/ml
	CAL2	0.20000	uIU/ml
	CAL3	5.00000	uIU/ml
	CAL4	25.00000	uIU/ml
	CAL5	50.00000	uIU/ml
	CAL6	100.00000	uIU/ml







<CALIB REQUEST (Conc. Set) Screen>

(6) Press  if the correct concentration is displayed. Otherwise, change the concentration.

Changing Concentration

<1> Use   to move the cursor to CAL and

press .

This displays the Conc. Input screen.

ANALYTE	CAL	CONC	UNIT
#TSH	CAL1	0.00000	uIU/ml
	CAL2	0.20000	uIU/ml
	CAL3	5.00000	uIU/ml
	CAL4	25.00000	uIU/ml
	CAL5	50.00000	uIU/ml
	CAL6	100.00000	uIU/ml







<2> Press  to clear the concentration and enter the new concentration (shown on calibrator bottle).

<3> Press  to redisplay the CALIB REQUEST (Conc. Set) screen.

#TSH	CAL6	100.00000
100.00000		
7	8	9
4	5	6
1	2	3
0	.	+/-






<Conc. INPUT Screen>

<4> Confirm that the concentration has changed in the CALIB REQUEST (Conc. Set) screen then press

.

#TSH	CAL6	100.00000
110		
7	8	9
4	5	6
1	2	3
0	.	+/-






5.1. Generating Calibration Curves

(7) This displays the CALIB REQUEST (analyte set) screen. Install the calibrator and reagent cup while confirming progress on the screen.

← CALIB REQUEST

ANALYTE CHECK

POS	CONC.	ANALYTE
1 CAL1	0.00000 uIU/ml	#TSH
2		#TSH
3		#TSH
4 CAL2	0.20000 uIU/ml	#TSH
5		#TSH
6		#TSH

OK

CANCEL

Point

Press to display the next screen and move the carousel to the next position.

← CALIB REQUEST

ANALYTE CHECK

POS	CONC.	ANALYTE
7 CAL3	5.00000 uIU/ml	#TSH
8		#TSH
9		#TSH
10 CAL4	25.00000 uIU/ml	#TSH
11		#TSH
12		#TSH

OK

CANCEL

-
- Calibration measures each concentration three times.
 - **Calibrators must be positioned in order of concentration, starting from the lowest one.**
 - Reagent cups are positioned in sequence without empty slots in between.

← CALIB REQUEST

ANALYTE CHECK

POS	CONC.	ANALYTE
13 CAL5	50.00000 uIU/ml	#TSH
14		#TSH
15		#TSH
16 CAL6	110.00000 uIU/ml	#TSH
17		#TSH
18		#TSH

OK

CANCEL

< CALIB REQUEST (analyte set) Screen >

5.1. Generating Calibration Curves

5.1.2. Performing Calibration


- (1) Load the calibrator and reagent cup and press



If Diluent, Wash, or Substrate ran short at a calibration, the calibration should be redone to obtain an accurate result.


Please be sure to check the residual quantity of Diluent, Wash, or Substrate before requesting calibration.

- (2) This displays the CALIB REQUEST (Check Start) screen.

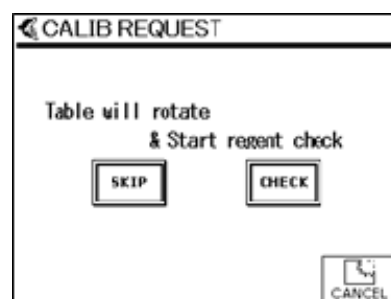

<CALIB REQUEST(Check Start) Screen>

- (3) Press  to rotate the carousel and check the positioning of calibrators and reagent cups. This displays the "Calibrator & Analyte Check 1" screen.

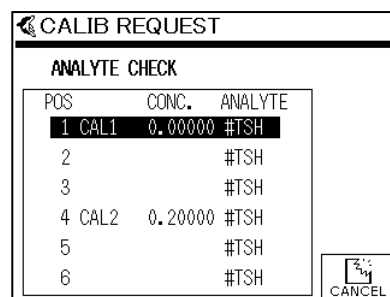

<CALIB REQUEST(Analyte Check 1) Screen>

Point

- Move the cursor to the CAL being checked.
- This highlights the selected CAL.
- Checking takes approximately 2 minutes for a two-point calibration, five minutes for a six-point calibration and seven minutes for a combined two-point and six-point calibration.
- Press  to skip the calibrator and reagent cup check and go on to the CALIB REQUEST (Analyte Check 2) screen.

5.1. Generating Calibration Curves

Errors

Errors occur when the calibrator position is wrong, the calibrator is missing or when the reagent cup analyte or lot numbers are wrong.

- <1> Errors are displayed on the CALIB REQUEST (Analyte Check 1) screen.

Point

The cursor stops at the location of the error.

CALIB REQUEST		
ERROR		
POS	CONC.	ANALYTE
1 CAL1	0.00000	#TSH
2		#TSH
3		#TSH
4 CAL2	0.20000	#TSH
5		#TSH
6		#TSH
		CANCEL

<ERROR Screen (Sample) >

- <2> Pressing  redisplay the CALIB REQUEST (Conc. Set) screen.

CALIB REQUEST			
ANALYTE	CAL	CONC	UNIT
#TSH	CAL1	0.00000	uIU/ml
	CAL2	0.20000	uIU/ml
	CAL3	5.00000	uIU/ml
	CAL4	25.00000	uIU/ml
	CAL5	50.00000	uIU/ml
	CAL6	110.00000	uIU/ml
			MODIFY
			OK
			CANCEL

<CALIB REQUEST(Conc. Set) Screen>

- <3> Reload the calibrator and reagent cups correctly and check again.



Placing the calibrators in a wrong concentration order will not result in an error message.

Position the calibrators in order of concentration, from the lowest to the highest.

- (4) When loaded correctly, the CALIB REQUEST (Analyte Check 2) screen appears.

- (5) Press the  key to start the calibration.

CALIB REQUEST		START
*** Calibration start ***		
Push [START] key		
		CANCEL

<CALIB REQUEST (Analyte Check 2) Screen>



Do not depress the START key for a long time.

Depressing the START key for a long time (about two seconds or longer) sends an abort request for an emergency stop and prints a warning message.

5.1. Generating Calibration Curves



If a warning message occurs indicating that daily check has not been performed, refer to "Chapter 4-2. System Startup" and follow the procedure.

[Screens Displayed During Calibration]

ASSAY MONITOR SEARCH	
01CAL1	#TSH
04CAL2	#TSH

Navigation: [Up] [Down] [Left] [Right] | END POS: 18 | [SUBSTRATE] [SAMP.ID]

ASSAY MONITOR WARMUP	

Navigation: [Up] [Down] [Left] [Right] | END POS: [] | [SUBSTRATE] [SAMP.ID]



Sample measurement cannot be performed during calibration.

ASSAY MONITOR SEARCH	
01 CAL1	#TSH

Navigation: [Up] [Down] [Left] [Right] | END POS: 18 | [SUBSTRATE] [SAMP.ID]

ASSAY MONITOR CALIB	
01CAL1	#TSH
04CAL2	#TSH
07CAL3	#TSH
10CAL4	#TSH
13CAL5	#TSH
16CAL6	#TSH

Navigation: [Up] [Down] [Left] [Right] | END POS: 18 | [SUBSTRATE] [SAMP.ID]

ASSAY MONITOR STOP	
01CAL1	#TSH
04CAL2	#TSH
07CAL3	#TSH
10CAL4	#TSH
13CAL5	#TSH
16CAL6	#TSH

Navigation: [Up] [Down] [Left] [Right] | END POS: [] | [SUBSTRATE] [SAMP.ID]

- (6) When the calibration is complete, the CALB displayed at the top right of the screen changes to STOP.

5.2. Reviewing/Updating New Calibration Curves

5.2.1. Calibration Review


The first assay result is output approximately 20 minutes after the assay operation begins, result reports appear every 100 sec thereafter.

Review and calculations using the calibration data should be conducted when calibration is complete.

Calibration data can be reviewed using the CALIB REVIEW screen.


Procedures

- (1) Press the **MENU** key to display the MENU screen.

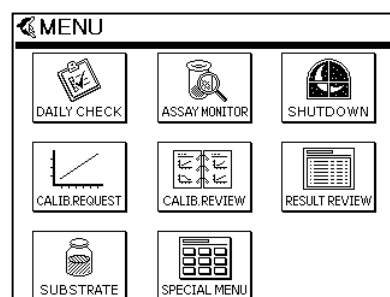

<MENU Screen>

- (2) Press  to display the CALIB REVIEW screen.

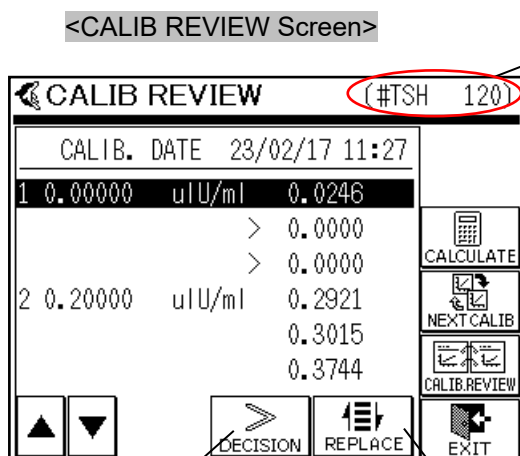

<CALIB REVIEW Screen>

Item and Lot no.

Calculates Calibration Curve
Moves to <CALIB ACCEPT Screen>.

Displays unreviewed calibration data
in sequence.

Displays list of reviewed calibrations.
Moves to <CALIB REVIEW LIST
Screen>.

Assigns accept and do not accept
flags to each value.

Sort RATE values in ascending/descending
order.
Moves to <CALIB REPLACE Screen>.

5.2. Reviewing/Updating New Calibration Curves

(3) The system is designed so that all unflagged assay results that appear when the screen is displayed are accepted. In order to delete data inappropriate for the calibration

calculations, use   to move the cursor to the inappropriate value and press  to reject.

Point


To accept the rejected data item, simply press  to toggle.

Point

If the calibrators are positioned in a wrong order and assays are performed, the RATE values can be sorted in ascending/descending order.

To Sort the RATE Values

(1) Press  on the CALIB REVIEW screen.
The CALIB REPLACE screen appears.

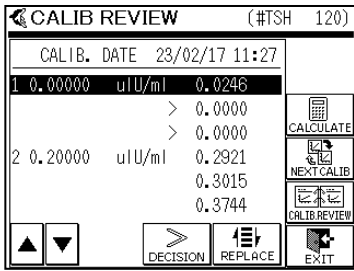

CALIB REVIEW		(#TSH 120)
CALIB. DATE 23/02/17 11:27		
1	0.00000 uIU/ml	0.0246
	>	0.0000
	>	0.0000
2	0.20000 uIU/ml	0.2921
		0.3015
		0.3744

Controls:        

<CALIB REVIEW Screen>

(2) Press  to select the sort order.
Ascending order: INCREASE RATE ORDER
Descending order: DECREASE RATE ORDER



INCREASE RATE ORDER
DECREASE RATE ORDER

Controls:   

<CALIB REPLACE Screen>



The initial cursor position on the CALIB REPLACE screen is different depending on the calibration curve type of each analyte.

(3) Press  to sort the order and return to the CALIB REVIEW screen.


(4) Press  to return to the CALIB REVIEW screen without sorting the order.



If the RATE values cannot be sorted, a warning message appears.

5.2. Reviewing/Updating New Calibration Curves

- (4) Once assay results have been reviewed, click .
This displays the CALIB ACCEPT screen.

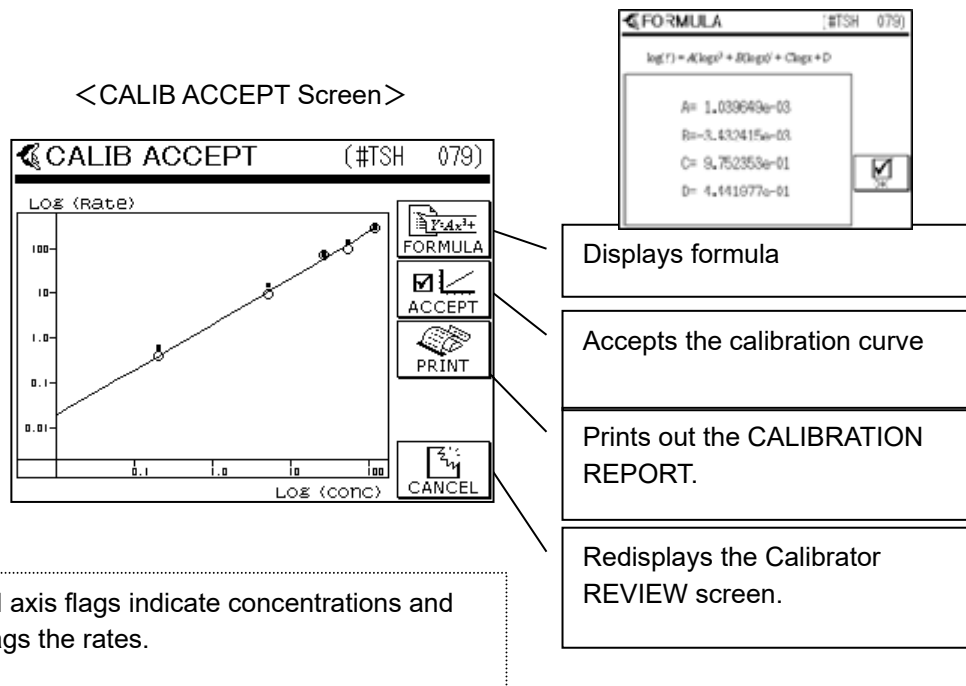

Point

Calibrations displayed in the CALIBRATION ACCEPT screen can be recalculated

repeatedly until  (calibration verify) is pressed.

5.2. Reviewing/Updating New Calibration Curves

5.2.2. Verifying Calibration Curves

The calibration curves are verified once calibration results have been reviewed.



Note that assay data cannot be changed or recalculated once verification has been performed.


Point

- The maximum number of lots verifiable per analyte is two.
- The same lot cannot be verified.

Procedures

Go to the CALIB ACCEPT screen

- (1) Press  to review the calibration curves.

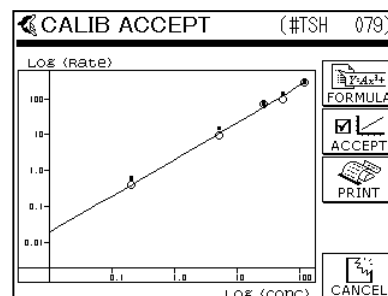

- (2) A CALIBRATION REPORT will be printed out.

Fig. 5 - 1 Sample Printout

Formula
Calibration flag

Concentrations

Rates

Coefficients

```

*** CALIBRATION REPORT ***
OP: 03/11/20
CalDate: 03/11/20
Status: ACCEPT
Analyte : *TSH Lot : 79

log(Y) = A(logx)2 + B(logx) + Clogx + D

Log(Rate)
100
10
1.0
0.1
0.01
0.1 1.0 10 100
Log(Conc)


Conc1=0.00000
Conc2=0.20000
Conc3=5.00000
Conc4=25.00000
Conc5=50.00000
Conc6=110.00000
Rate1=0.00000000
Rate2=0.397185507
Rate3=9.700236320
Rate4=72.839823814
Rate5=94.284044495
Rate6=295.383005371
Func[A]= 2.101968e-03
Func[B]= 1.129584e-02
Func[C]= 1.017185e+00
Func[D]= 3.046034e-01
***END***
  
```

5.2. Reviewing/Updating New Calibration Curves

(3) Any unverified calibration curves can be displayed by calling up the CALIB REVIEW screen.

Point


To delete unverified calibration curves, press  select the calibration curve on the CALIB REVIEW LIST screen and press .

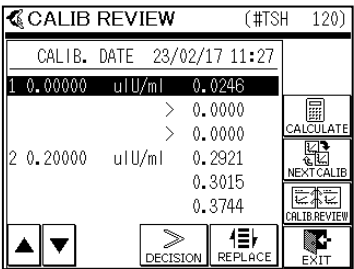

<CALIB REVIEW Screen>


(4) The CALIBRATION REVIEW LIST screen is displayed when all calibration curves have been verified.

<CALIB REVIEW LIST Screen>

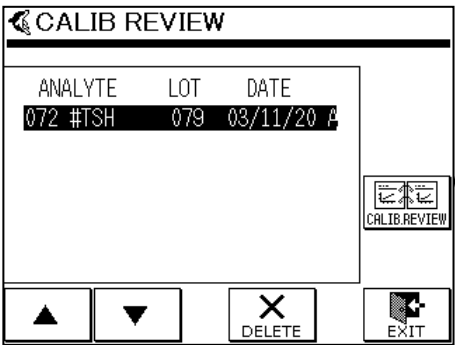


Deletes calibration curve.

Displays the CALIB. REVIEW screen.

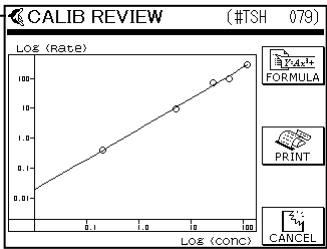

Chapter 6: Assay Procedures

6.0. Introduction

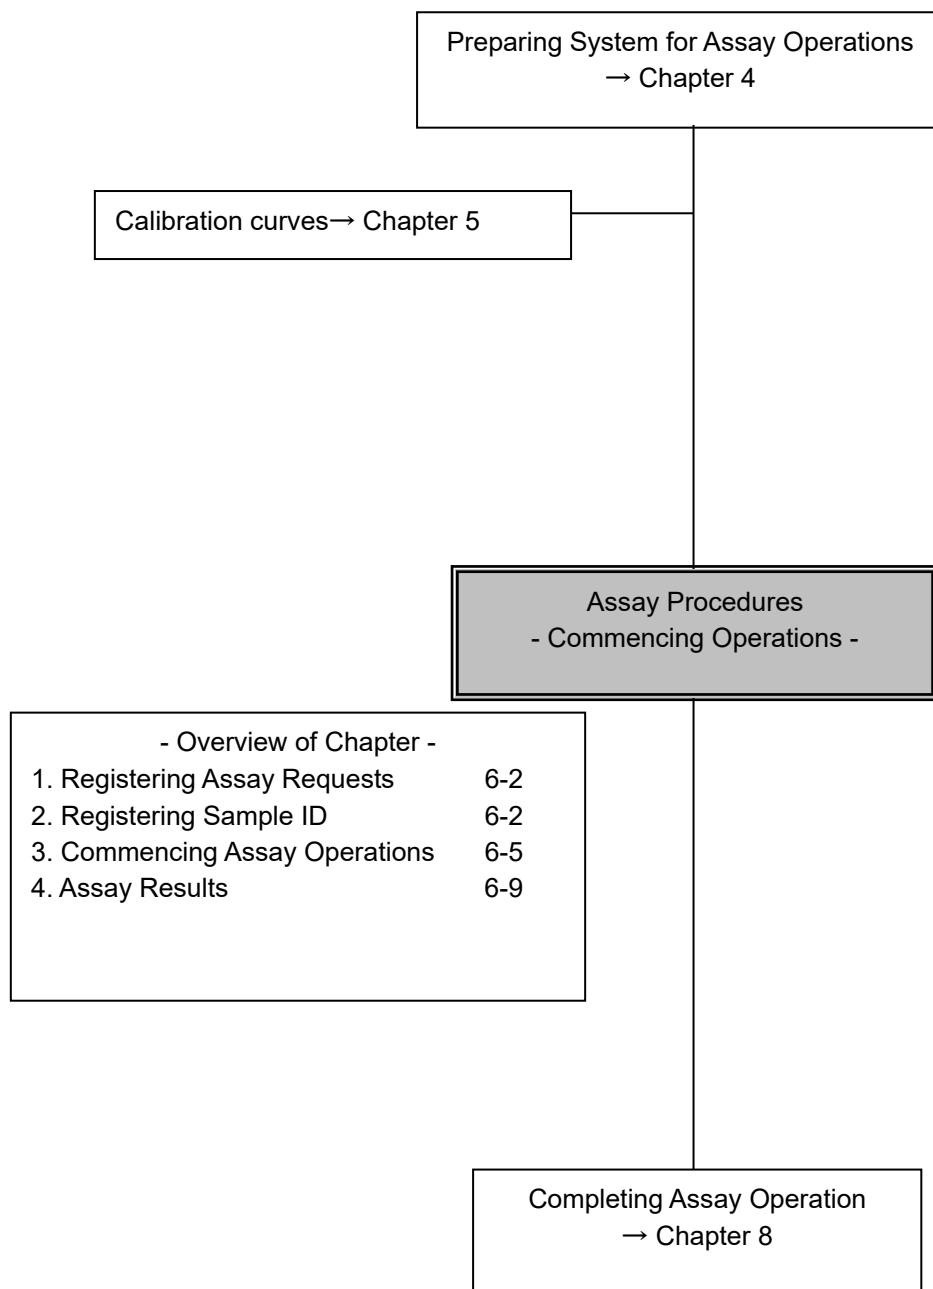

6.1. Registering Assay Requests

Assay requests are registered automatically using the combination of an internal barcode reader and a cup reader.

The AIA-360 is equipped with a camera capable of reading analyte names and lot numbers, enabling it to automatically distinguish between specimen types and select the appropriate assay operations, as soon as specimens and reagent cups are loaded in the carousel.

Point

- **Note that up to four tests can be performed per specimen. This means that the fifth and all subsequent reagent cups per specimen will be skipped.**
- **In cases where tests are performed using designated sample cups, sample IDs will be assigned in the order SMPL1, SMPL2, SMPL3, etc.**

6.2. Registering Sample ID

AIA-360 automatically registers a sample's ID using the built-in barcode reader.

The ID of an arbitrary sample can be registered by entering a sample ID before starting an assay.

The sample ID registration conditions are as follows:

Sample Container	Arbitrary Sample ID	
	Input	No Input
Sample cup	Entered ID is registered.	Auto registration (SMPL1, SMPL2, SMPL3, ...)
Blood tube with no barcode label	Entered ID is registered.	Auto registration (SMPL1, SMPL2, SMPL3, ...)
Blood tube with barcode label	Entered ID is registered if it matches the sample ID read by the built-in barcode reader. If they do not match, an IM flag is attached with no assay.	Auto registration (Sample ID on barcode label)


For the settings of the built-in barcode reader, see **Chapter 9 “OTHER FUNCTIONS - SPECIAL, MENU - 6. BCR PARAM (DETAILED SETTINGS OF BARCODE)”**.

6.2.1. Entering a sample ID



**Enter a sample ID before the sample passes the built-in barcode reader.
Once a sample has passed the barcode reader, its ID cannot be entered.**


- (1) Press  on the ASSAY MONITOR screen.
The SAMPLE ID LIST screen is displayed.

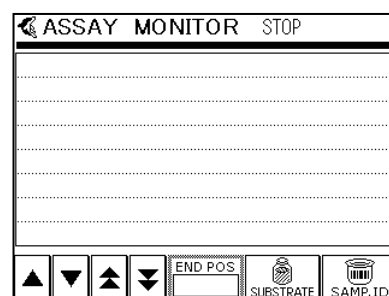

<ASSAY MONITOR Screen>

- (2) Move the cursor to the sample ID to be inputted by using   and then press .

The SAMPLE ID screen is then displayed.

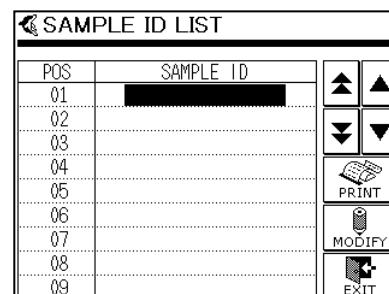

<SAMPLE ID LIST Screen>

6.2. Registering Sample ID


(3) Enter a sample ID (16 digits max.).

Pressing  changes the mode as follows:

 Alphabetic characters (uppercase)

 Alphabetic characters (lowercase)


 Numerals and/or symbols

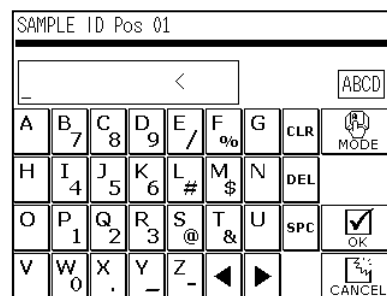

The screen displays 'SAMPLE ID Pos 01' at the top. Below it is a large input field with a left arrow. To the right of the input field is a button labeled 'ABCD'. Below the input field is a grid of buttons: A, B, C, D, E, F, G, CLR, and a button with a hand icon labeled 'MODE'. The second row contains H, I, J, K, L, M, N, DEL, and a button with a checkmark labeled 'OK'. The third row contains O, P, Q, R, S, T, U, SPC, and a button with a checkmark labeled 'OK'. The bottom row contains V, W, X, Y, Z, a left arrow, a right arrow, and a button labeled 'CANCEL'.

<SAMPLE ID Screen>

(4) After inputting, press  to return to the SAMPLE ID LIST screen.

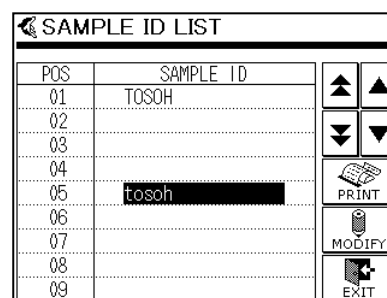

The screen displays 'SAMPLE ID LIST' at the top. Below it is a table with two columns: 'POS' and 'SAMPLE ID'. The table contains 9 rows. The first row has '01' in the 'POS' column and 'TOSOH' in the 'SAMPLE ID' column. The second row has '02' in the 'POS' column and an empty 'SAMPLE ID' field. The third row has '03' in the 'POS' column and an empty 'SAMPLE ID' field. The fourth row has '04' in the 'POS' column and an empty 'SAMPLE ID' field. The fifth row has '05' in the 'POS' column and 'tosoh' in the 'SAMPLE ID' column. The sixth row has '06' in the 'POS' column and an empty 'SAMPLE ID' field. The seventh row has '07' in the 'POS' column and an empty 'SAMPLE ID' field. The eighth row has '08' in the 'POS' column and an empty 'SAMPLE ID' field. The ninth row has '09' in the 'POS' column and an empty 'SAMPLE ID' field. To the right of the table are four buttons: a left arrow, a right arrow, a button with a hand icon labeled 'PRINT', and a button with a hand icon labeled 'MODIFY'. At the bottom right is a button labeled 'EXIT'.


<SAMPLE ID LIST Screen>

Point

Pressing  prints a sample ID list.

To prevent mistakes from occurring, check the sample ID list when loading samples.

(5) After checking that a sample ID has been entered, press

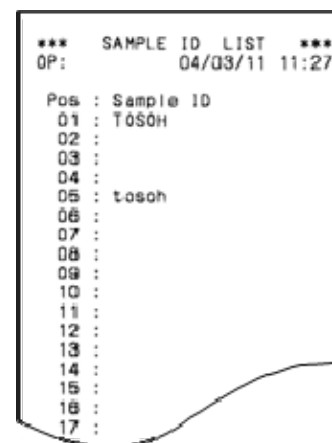The screen displays a printed list of sample IDs. At the top, it says '*** SAMPLE ID LIST ***'. Below that, it says 'OP: 04/03/11 11:27'. The list is as follows:

```

Pos : Sample ID
01 : TOSOH
02 :
03 :
04 :
05 : tosoh
06 :
07 :
08 :
09 :
10 :
11 :
12 :
13 :
14 :
15 :
16 :
17 :
  
```

6.2. Registering Sample ID

- (6) When the ASSAY MONITOR screen is displayed, start inspection according to Section 3. “Commencing Assay Operations”.

← ASSAY MONITOR ASSAY		
01 TOSOH	#FT4	#FT3
05 tosoh	#T4	#FT3
	#FT4	#FT3
	#T4	#FT3

▲
▼
▲
▼

END POS
08


 SUBSTRATE


 SAMP. ID

<ASSAY MONITOR screen>

The built-in barcode reader reads a sample and the entered sample ID is registered.

Point

- After a sample has been read by the built-in barcode reader, the entered sample ID disappears from the SAMPLE ID LIST screen.
- An arbitrary sample ID can also be entered for additional assay.


6.3. Commencing Assay Operations

- (1) Assay operations begin with the loading of specimens and reagent cups into the carousel.

Test Tube (sample cup) and Reagent Cup Loading Procedure

Begin by loading test tubes (or designated sample cups) into the sample holder and reagent cups (numbers correspond to analytes) into the reagent cup holder.

Fig. 6-1 Test Tube and Reagent Cup Loading Procedure

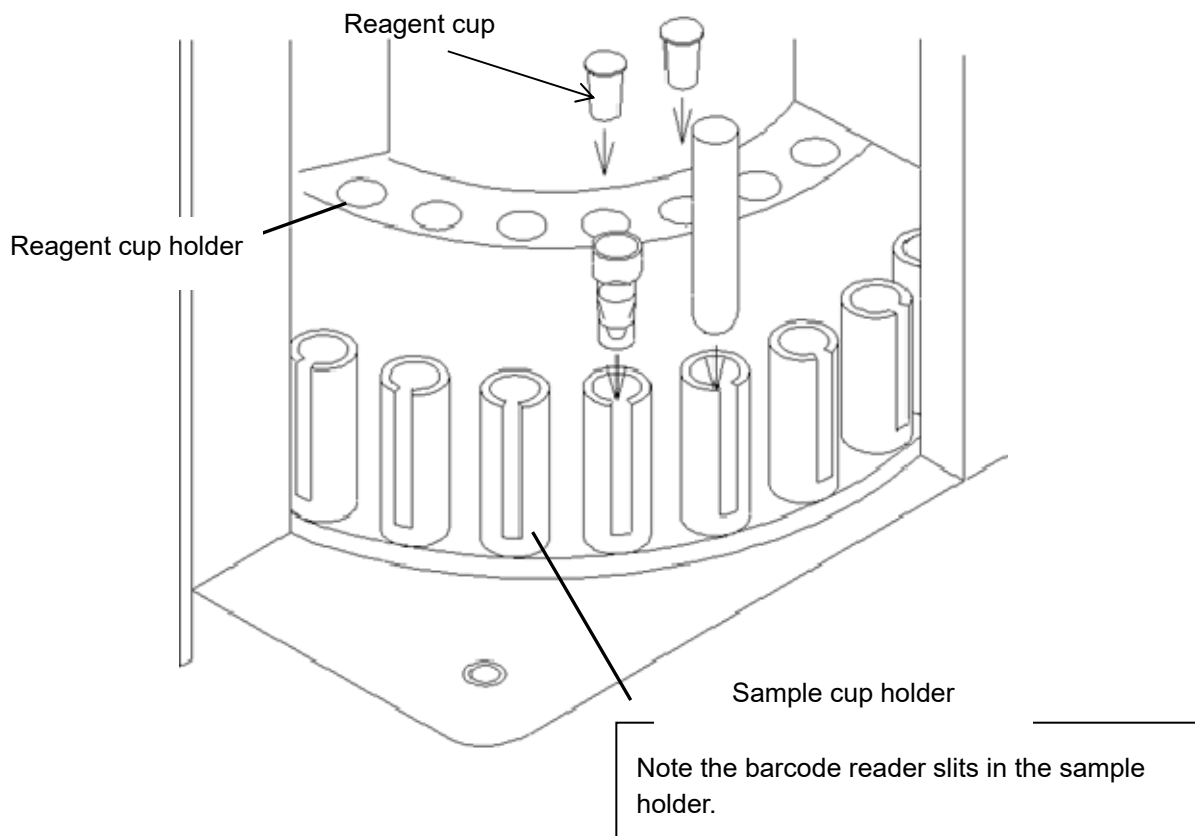


Point

- Up to four reagent cups can be assayed per specimen.
- To analyze multiple analytes per specimen, load the reagent cups at consecutive positions of the reagent cup holder, and load the specimen only at the first position of the corresponding sample cup holder.
- The carousel can be moved one position at a time by pressing the **SAMPLE FEED** key.

6.3. Commencing Assay Operations



- Before loading test tubes or other containers into the sample cup holder, be sure to remove their caps. If not, accurate results may not be obtained, and the instrument may be damaged.
- Make sure to firmly insert the test tubes (sample cups) and reagent cups into their holders. Loosely inserted cups can get caught when the carousel rotates and stops the assay operation.
- Be sure to position the bar codes at the sample holder slits when using test tubes with barcodes attached, so that they can be easily read.

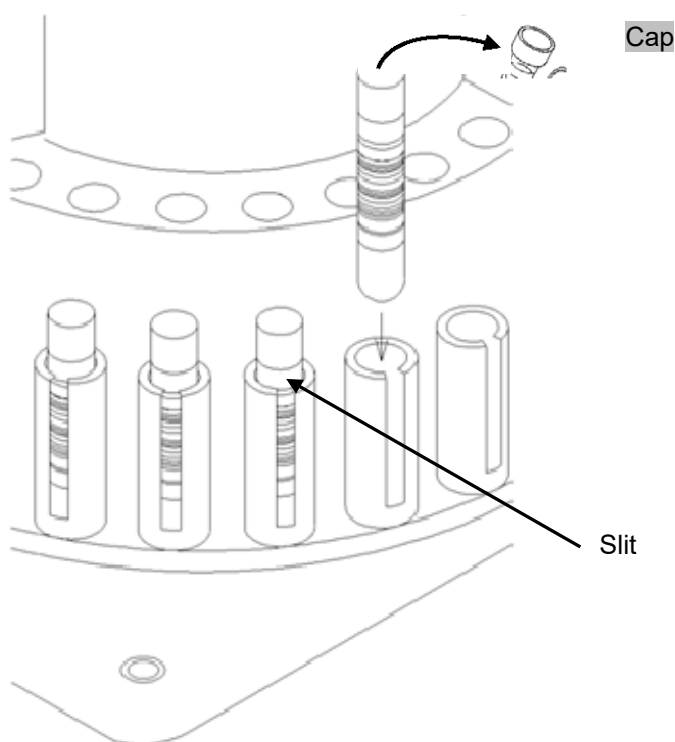


6.3. Commencing Assay Operations

- (2) Once the samples and reagent cups have been

loaded, press  on the MENU screen to display the ASSAY MONITOR screen.

- (3) Press **START** to start the assay operation.

The carousel moves in clockwise direction when the assay begins.

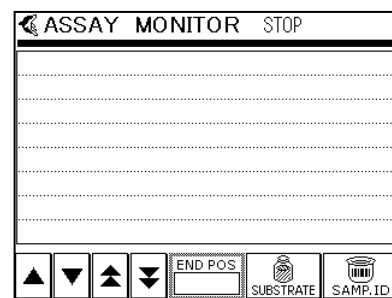

The screen displays "ASSAY MONITOR STOP" at the top. Below the title is a large empty rectangular area. At the bottom, there is a control bar with four arrow keys (up, down, left, right), a field labeled "END POS" with a value of "01", and two icons labeled "SUBSTRATE" and "SAMP.ID".

<ASSAY MONITOR Screen>



Do not depress the START key for a long time. Depressing the START key for a long time (about two seconds or longer) sends an abort request for an emergency stop and prints a warning message.



If a warning appears indicating that daily check has not been performed, refer to "Chapter 4-2. System Startup" and follow the procedure.




Note that pressing **SAMPLE FEED during the assay operation will not move the carousel forward.**

SAMPLE ID


Sample ID (up to 16 characters) can be displayed on the screen when the specimen is read.

ANALYTE


Analytes in the reagent cups read from the camera are displayed for each sample. (Maximum 4 tests)

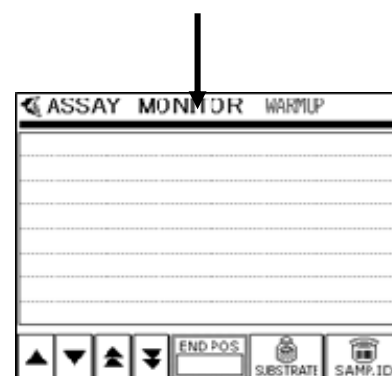

The screen displays "ASSAY MONITOR WARMUP" at the top. Below the title is a large empty rectangular area. At the bottom, there is a control bar with four arrow keys (up, down, left, right), a field labeled "END POS" with a value of "01", and two icons labeled "SUBSTRATE" and "SAMP.ID".

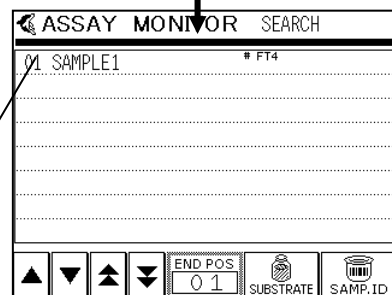

The screen displays "ASSAY MONITOR SEARCH" at the top. Below the title, it shows "01 SAMPLE1" and "# FT4". Below this is a large empty rectangular area. At the bottom, there is a control bar with four arrow keys (up, down, left, right), a field labeled "END POS" with a value of "01", and two icons labeled "SUBSTRATE" and "SAMP.ID".

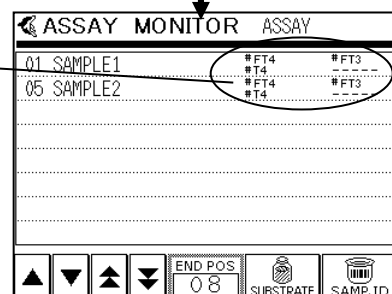

The screen displays "ASSAY MONITOR ASSAY" at the top. Below the title, it shows "01 SAMPLE1" and "# FT4" on the first line, and "05 SAMPLE2" and "# FT4" on the second line. To the right of these, there are two columns of test results labeled "# FT3" and "# FT4". Below this is a large empty rectangular area. At the bottom, there is a control bar with four arrow keys (up, down, left, right), a field labeled "END POS" with a value of "08", and two icons labeled "SUBSTRATE" and "SAMP.ID".



If a problem happens while assaying, press the START key for a long time (about two seconds or longer) to send an abort request, so an emergency stop occurs. Then a warning message will be printed.

6.3. Commencing Assay Operations

- (4) The carousel makes one more rotation after the reagent cup in the final position has been assayed.

↓

ASSAY MONITOR		SEARCH	
01	SAMPLE1	○ #FT4	○ #FT3
05	SAMPLE2	○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3

▲ ▼ ▲ ▼ END POS 08 SUBSTRATE SAMP.ID

- (5) Once it has confirmed that all reagent cups have been assayed, 'CLOSING' will be displayed on the upper right of a screen and it will go into end process.

After end process, 'STOP' is displayed and measurement is suspended.

↓

ASSAY MONITOR		STOP	
01	SAMPLE1	○ #FT4	○ #FT3
05	SAMPLE2	○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3
		○ #FT4	○ #T3
		○ #T4	○ #FT3

▲ ▼ ▲ ▼ END POS 08 SUBSTRATE SAMP.ID

- (6) Collect all the test tubes and sample cups after the assays are completed.
- The carousel can be moved one position at a time by pressing the SAMPLE FEED key.



If there is any test tube with its cap still attached when collecting sample containers, perform the assay again.

6.3. Commencing Assay Operations

Additional Assays

Additional assays can be added while assay operations are in progress by inserting them in the visible section of the carousel.

 Point

Additional assays may be added only while either “ASSAY” or “SEARCH” are displayed at the top right of the ASSAY MONITOR screen.

- <1> Make sure to remove any samples and reagent cups that have already been assayed at this time.
- <2> Then insert the additional samples and reagent cups in the visible section of the carousel.



The LED lamp begins flashing 10 seconds before the carousel begins to rotate. Take care not to get fingers caught in the carousel when inserting additional samples and reagent cups.

- <3> The new assays will be added automatically.


6.3. Commencing Assay Operations

Display of estimated end time of assay



When  on the ASSAY MONITOR screen is pressed during measurement, the screen is changed and the estimated end time of assay is displayed.

ASSAY MONITOR		ASSAY	
13	CAL5	○ MYO	○ MYO
16	CAL6	○ MYO	○ MYO
01	SAMPLE1	○ MYO	○ MYO
03	SAMPLE2	○ #TSH	<L MYO
05	SAMPLE3	#TSH	MYO
07	SAMPLE4	#TSH	MYO
09	SAMPLE5	MYO	#TSH
11	SAMPLE6	MYO	#TSH



ASSAY MONITOR		ASSAY	
13	CAL5	15:51 ○ MYO	○ MYO
16	CAL6	15:56 ○ MYO	○ MYO
01	SAMPLE1	○ #TSH	<L MYO
03	SAMPLE2	16:24 #TSH	MYO
05	SAMPLE3	16:27 #TSH	MYO
07	SAMPLE4	16:30 #TSH	MYO
09	SAMPLE5	16:34 #TSH	MYO
11	SAMPLE6	16:37 MYO	#TSH
		16:40 MYO	#TSH

Estimated end time of assay

Displays the estimated assay end time of the specimen.

Point



Press  to return to the previous display (to hide the time display on the screen).



Press  to show the time display on the screen.

6.4. Assay Results

6.4.1. External Output of Assay Results

- (1) Press  on the MENU screen to display the RESULT REVIEW screen.

RESULT REVIEW		
DATE 03/11/21 13:58 LOT 015 031/036		
SAMPLE1	#FT4	1.55
SAMPLE1	#FT3	2.75
SAMPLE1	#T4	1.7
SAMPLE2	#FT4	4.39
SAMPLE2	#FT3	9.44
SAMPLE2	#T4	16.7

RESULT REVIEW Screen>

- (2) Press  and use   to select the range of detailed Assay Results to output externally.
(Selected range is flagged by the + sign)

RESULT REVIEW		
DATE 03/11/21 13:58 LOT 015 031/036		
SAMPLE1	#FT4	1.55
+ SAMP1E1	#FT3	2.75
+ SAMP1E1	#T4	1.7
SAMPLE2	#FT4	4.39
SAMPLE2	#FT3	9.44
SAMPLE2	#T4	16.7

Point Press   to proceed to the next screen.

- (3) Press  to confirm the selected range.
(This changes the + signs to the > sign)

RESULT REVIEW		
DATE 03/11/21 13:58 LOT 015 031/036		
SAMPLE1	#FT4	1.55
> SAMP1E1	#FT3	2.75
> SAMP1E1	#T4	1.7
SAMPLE2	#FT4	4.39
SAMPLE2	#FT3	9.44
SAMPLE2	#T4	16.7

Point To deselect the specified range, press .

- (4) Next, press .

- (5) This displays the RESULT EXECUTE screen.

RESULT EXECUTE		
		
TRANSMIT	PRINT	RECALC.
		
CANCEL		

<RESULT EXECUTE Screen>

- (6) Pressing the  displays the RESULT REVIEW screen and the selected range of Assay Results is output externally.

6.4. Assay Results

6.4.2. Printing Assay Results

- (1) Press  on the MENU screen to display the RESULT REVIEW screen.

RESULT REVIEW		
DATE 03/11/21 13:56 LOT 015 031/036		
SAMPLE1	# FT4	1.55
SAMPLE1	# FT3	2.75
SAMPLE1	# T4	1.7
SAMPLE2	# FT4	4.39
SAMPLE2	# FT3	9.44
SAMPLE2	# T4	16.7

<RESULT REVIEW Screen>

- (2) Press  and use   to select the range of detailed Assay Results to output externally. (Selected range is flagged by the + sign)

RESULT REVIEW		
DATE 03/11/21 13:56 LOT 015 031/036		
SAMPLE1	# FT4	1.55
+ SAMP1E1	# FT3	2.75
+ SAMP1E1	# T4	1.7
SAMPLE2	# FT4	4.39
SAMPLE2	# FT3	9.44
SAMPLE2	# T4	16.7

Point Press   to proceed to the next screen.

- (3) Press  to confirm the selected range. (This changes the + signs to the > sign)

RESULT REVIEW		
DATE 03/11/21 13:56 LOT 015 031/036		
SAMPLE1	# FT4	1.55
> SAMP1E1	# FT3	2.75
> SAMP1E1	# T4	1.7
SAMPLE2	# FT4	4.39
SAMPLE2	# FT3	9.44
SAMPLE2	# T4	16.7

Point To deselect the specified range, press .


- (4) Next, press .

- (5) This displays the RESULT EXECUTE screen.

- (6) Press  to print out the selected range of Assay Results.

RESULT EXECUTE		
 TRANSMIT	 PRINT	 RECALC.
 CANCEL		

<RESULT EXECUTE Screen>

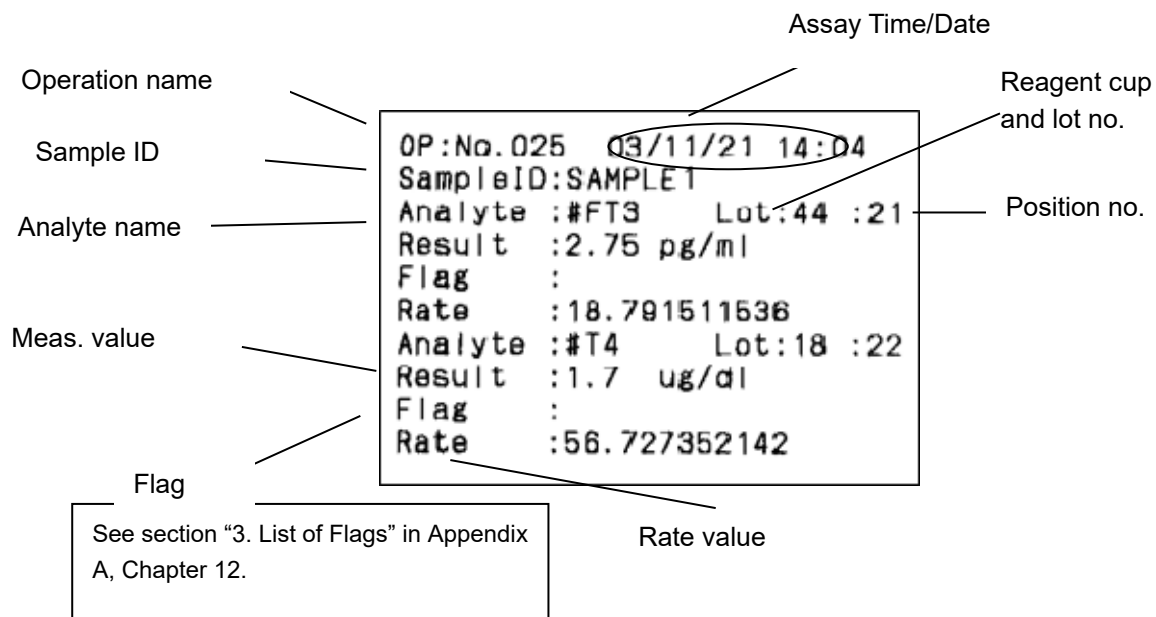6.4. Assay Results**Fig. 6-2 Sample Assay Result Printout**

6.4. Assay Results

6.4.3. Recalculating Assay Results

- (1) Press  on the MENU screen to display the RESULT REVIEW screen.

RESULT REVIEW		
DATE 03/11/21 13:56 LOT 015 031/036		
SAMPLE1	# FT4	1.55
SAMPLE1	# FT3	2.75
SAMPLE1	# T4	1.7
SAMPLE2	# FT4	4.39
SAMPLE2	# FT3	9.44
SAMPLE2	# T4	16.7

- (2) Press  and use   to select the range of detailed Assay Results to output externally.
(Selected range is flagged by the + sign)

<RESULT REVIEW Screen>

RESULT REVIEW		
DATE 03/11/21 13:56 LOT 015 031/036		
SAMPLE1	# FT4	1.55
+ SAMPLE1	# FT3	2.75
+ SAMPLE1	# T4	1.7
SAMPLE2	# FT4	4.39
SAMPLE2	# FT3	9.44
SAMPLE2	# T4	16.7

Point

- Press   to proceed to the next screen.

6.4. Assay Results

- (3) Press  to confirm the selected range.
(This changes the + signs to the > sign)

Point

To deselect the specified range, press .

- (4) Next, press .
This displays the RESULT EXECUTE screen.

RESULT REVIEW			
DATE 03/11/21 13:56 LOT 015 031/036			
SAMPLE1	# FT4	1.55	
> SAMP1E1	# FT3	2.75	
> SAMP1E1	# T4	1.7	
SAMPLE2	# FT4	4.39	
SAMPLE2	# FT3	9.44	
SAMPLE2	# T4	16.7	

RESULT EXECUTE			
 TRANSMIT	 PRINT	 RECALC.	
			 CANCEL

<RESULT EXECUTE Screen>

- (5) Pressing  recalculates the selected range of Assay Results.

Chapter 7: Error Messages and Flags

7.1. List of Error Messages

If a problem occurs during assay or it is difficult to continue an assay, an error message is displayed.

Together with the error message, a buzzer sounds to alert the operator to the error.

At the same time, the printer also prints the error message.



If an assay is not completed normally due to an error, an error flag may be attached to the assay value.

7.1.1. Error Message Lists

When an assay is started soon after turning the power switch on, if the incubator has not reached the appropriate temperature, Error Message No. 3003 is displayed and the assay may not be started.

No.	Error Message	Meaning	Troubleshooting
3003	WAITING FOR TEMPERATURE	Waiting for the temperature to rise.	Wait until the temperature rises to correct temperature.

7.1. List of Error Messages

If one of Error Messages No. 3017 to 3020 is displayed, the assay is suspended. If a reaction is in progress, however, the assay continues. Take the appropriate action in accordance with the displayed message and restart the assay. After all the ongoing assays end, perform the corresponding troubleshooting and press the START key to restart assays.

No.	Error Message	Meaning	Troubleshooting
3017	SUBSTRATE LOW	Insufficient substrate.	After confirming that 'ASSAY' displayed on the upper right of the ASSAY MONITOR screen changes to 'STOP', replace the enzyme substrate with new one and press the START key to restart assay operation.
3018	WASTE TANK FULL	The waste tank is full.	After confirming that 'ASSAY' displayed on the upper right of the ASSAY MONITOR screen changes to 'STOP', empty the waste tank and press the START key to restart assay operation.
3019	WASHER LOW	Insufficient wash solution.	After confirming that 'ASSAY' displayed on the upper right of the ASSAY MONITOR screen changes to 'STOP', replace the wash solution with new one and press the START key to restart assay operation.
3020	DILUENT LOW	Insufficient diluent.	After confirming that 'ASSAY' displayed on the upper right of the ASSAY MONITOR screen changes to 'STOP', replenish the diluent and press the START key to restart the assay operation

7.1. List of Error Messages

If an error occurs, the device stops and the message shown below is displayed.
If an error message is displayed during an assay, you may not be able to continue the assay.

Operating Errors

No.	Error message	Description	Troubleshooting
0001	FILE SYSTEM ERROR	The external recording medium could not be initialized.	Use other media or contact the local Tosoh representative.
0002	MAIN PROGRAM OPEN ERROR	The main program cannot be read.	Use other media or contact the local Tosoh representative.
0003	MAIN PROGRAM FORMAT ERROR	The file format of the main program is incorrect.	Use other media or contact the local Tosoh representative.
0004	SLAVE PROGRAM OPEN ERROR	The slave program cannot be read.	Use other media or contact the local Tosoh representative.
0005	SLAVE PROGRAM FORMAT ERROR	The file format of the slave program is incorrect.	Use other media or contact the local Tosoh representative.
0006	TOUCH PANEL PROGRAM OPEN ERROR	The touch panel program cannot be read.	Use other media or contact the local Tosoh representative.
0007	INSTALLATION OPEN ERROR	The image data cannot be read.	Use other media or contact the local Tosoh representative.
0008	INSTALLATION FORMAT ERROR	The format of the image data file is incorrect.	Use other media or contact the local Tosoh representative.
0009	INSUFFICIENT STANDARD CUP	No standard cup is loaded for the daily check.	Load a standard cup on reagent cup holder No.1 and repeat.
0010	TWO CALIBRATION CURVES CONFIRMED	Calibration curves of two lots have already been confirmed.	Delete a calibration curve before accepting a new one.
0011	SAME LOT CALIBRATION CURVE	Calibration curves have already been confirmed for the same lot.	Delete the old calibration curve before accepting a new one.
0012	CALIBRATION NOT ENOUGH	There is insufficient data to calculate calibration curves.	Repeat the calibration.
0013	CALCULATION ERROR	Calculation error of the calibration curve.	Repeat the calibration.
0014	CALIBRATION DATA ZIGZAG	The calibration curve rates are not in ascending order.	Repeat the calibration.
0015	TOO MANY CALIBRATION DATA	The calibration curve data is abnormal.	Repeat the calibration.
0016	CALIBRATION DATA MINUS RATE	Logarithm calculation of calibration curve failed.	Repeat the calibration.
0017	TOMAS DATA WRITE ERROR	Unable to write external recording medium.	Use other media or contact the local Tosoh representative.

7.1. List of Error Messages

Communication-related errors

No.	Error message	Description	Troubleshooting
1001	UNABLE TO SEND TO SLAVE	FIFO has become full during transmission to the slave.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
1002	UNABLE TO RECEIVE FROM SLAVE	A communication error occurred during transmission to the slave.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
1003	RECEIVE DATA ERROR FROM T.PANEL	A communication error occurred during reception from the touch panel.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
1004	TRANSMISSION TO T.PANEL TIMED OUT	A timeout error occurred during reception from the touch panel.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
1005	BARCODE ERROR	A barcode communication error occurred.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
1006	ASTM PARITY ERROR	A parity error occurred in ASTM communication.	Check the communication settings and cable.
1007	ASTM FRAME ERROR	An ASTM communication frame error occurred.	Check the communication settings and cable.
1008	ASTM OVERRUN ERROR	ASTM communication overrun error	Check the communication settings and cable.
1009	ASTM BUFFER FULL	The ASTM communication buffer has become full.	Check the communication settings and cable.
1011	ASTM RETRY ERROR	An ASTM communication retry error occurred.	Check the communication settings and cable.
1012	ASTM SEND TIMEOUT	A send timeout event occurred in ASTM communication.	Check the communication settings and cable.
1013	ASTM RECEIVE TIMEOUT	A receive timeout error occurred in ASTM communication.	Check the communication settings and cable.
1014	ASTM NO RESPONSE	No response was received in ASTM communication.	Check the communication settings and cable.

Control related errors

No.	Error message	Description	Troubleshooting
2001	RTC POWER ON CLEAR	An internal clock backup error occurred.	Reset the date and time. If this problem reoccurs, contact the local Tosoh representative.
2002	TESTCUP READ ERROR	The test cup read error occurred.	If this problem reoccurs frequently, contact the local Tosoh representative.
2003	TESTCUP READ ERROR	The test cup position error occurred at the detector calibration.	Set the test cup to a right position.
2004	DET CALIB. TESTCUP READ ERROR	The test cup read error at the detector calibration.	Set the STD cup to a right position.
2005	DET CALIB. DIVIDE BY ZERO	Data error at the detector calibration.	Check the conditions, Repeat the detector calibration.
2006	DET CALIB. DATA VARIANCE ERROR	Data variance error at the detector calibration.	Check the conditions, Repeat the detector calibration.
2007	DET CALIB. ABNORMAL DATA	Data abnormal error at the detector calibration.	Check the conditions, Repeat the detector calibration.

7.1. List of Error Messages

Control related errors

No.	Error message	Description	Troubleshooting
2008	DET CALIB. SUBSTRATE HB	The background intensity of substrate is high	Replace the new substrate
2009	BF PROBE LIQUID SENSOR ERROR	Liquid detection error in BF probe	Contact the local Tosoh representative.
2010	SAMPLE LEVEL FAILURE	A liquid detection open-circuit error occurred at the sample nozzle.	Contact the local Tosoh representative.
2011	AIR DETECTED [SAMPLE]	There is no contact with the liquid surface after sample suction.	Contact the local Tosoh representative.
2012	AIR DETECTED [DILUENT]	There is no contact with the liquid after diluent suction.	Contact the local Tosoh representative.
2013	SAMPLE LEVEL DETECTION ERROR	The liquid surface cannot be detected even at the bottom of the sample cup or the blood sample tube.	Contact the local Tosoh representative.
2014	SAMPLE SHORTAGE DETECTED	Insufficient sample.	Prepare enough volume of specimen.
2015	BF PROBE PURGE FAILURE	Purging by the BF probe is abnormal.	Clean up the wash probe tip or replace it. Contact the local Tosoh representative.
2016	BF PROBE SUCTION FAILURE	Suction by the BF probe is abnormal.	Contact the local Tosoh representative.
2017	SUBSTRATE PURGE FAILURE	The substrate was not purged normally.	Check for insufficient substrate.

Monitor-related errors

No.	Error message	Description	Troubleshooting
3001	PRINTER PAPER END	No paper is loaded in the printer.	Load paper in the printer.
3002	PRINTER HEAD UP	The printer head has gone up.	Lower the printer head.
3003	WAITING FOR TEMPERATURE	Waiting for the temperature to rise.	Wait until the temperature rises to correct temperature.
3004	TEMPERATURE TIME OUTED	A timeout error occurred while waiting for the temperature to rise.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3005	TURN TABLE TEMPERATURE LOW	The turntable temperature is below the lower limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3006	WASHER TEMPERATURE LOW	The wash solution temperature is below the lower limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3007	SUBSTRATE TEMPERATURE LOW	The substrate temperature is below the lower limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3008	TURN TABLE TEMPERATURE HIGH	The turntable temperature is above the upper limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3009	WASHER TEMPERATURE HIGH	The wash solution temperature is above the target temp.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

7.1. List of Error Messages

Monitor-related errors

No.	Error message	Description	Troubleshooting
3010	SUBSTRATE TEMPERATURE HIGH	The substrate temperature is above the upper limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3011	TURN TABLE TEMP. MALFUNCTION	The turntable temperature sensor disconnection occurred.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3012	WASHER TEMP. MALFUNCTION	The wash solution temperature sensor disconnection occurred.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3013	SUBSTRATE TEMP. MALFUNCTION	The substrate temperature disconnection error occurred.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3014	TURN TABLE TEMP. LIMIT	The turntable temperature is above the upper limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3015	WASHER TEMP. LIMIT	The wash solution temperature reached the upper limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3016	SUBSTRATE TEMP. LIMIT	The substrate temperature is above the upper limit.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
3017	SUBSTRATE LOW	Insufficient substrate.	Replace the enzyme substrate.
3018	WASTE TANK FULL	The waste tank is full.	Empty the waste tank.
3019	WASHER LOW	Insufficient wash solution.	Replenish the wash solution.
3020	DILUENT LOW	Insufficient diluent.	Replenish the diluent.
3021	LEAK SENSOR S701 DETECTED	Leakage sensor S701 activated.	Contact the local Tosoh representative.
3022	LEAK SENSOR S702 DETECTED	Leakage sensor S702 activated.	Contact the local Tosoh representative.
3023	PM DUE	Periodic Maintenance due	Contact the local Tosoh representative.
3024	PM REQUIRED	Periodic Maintenance is required	Contact the local Tosoh representative.

Actuator-related errors

No.	Error message	Description	Troubleshooting
4001	TURN TABLE HOME SENSOR	The turntable motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4002	TURN TABLE HOME NOT FOUND	The home position of the turntable motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4003	TURN TABLE HOME OVERRUN	The turntable motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4004	TURN TABLE SLIP	The turntable motor slipped.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4005	TURN TABLE ACCELL	The acceleration/deceleration table of the turntable motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4006	TURN TABLE S106	The turntable anti-rotation sensor is activated.	Check that the blood sample tube is in contact with the sensor.

7.1. List of Error Messages

Actuator-related errors

4007	MIXER HOME SENSOR	The mixer motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4008	MIXER HOME NOT FOUND	The home position of the mixer motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4009	MIXER HOME OVERRUN	The mixer motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4010	MIXER SLIP	The mixer motor slipped.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4011	MIXER ACCELL	The acceleration/deceleration table of the mixer motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4012	SPEC.SY HOME SENSOR	The specimen syringe motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4013	SPEC.SY HOME NOT FOUND	The home position of the specimen syringe motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4014	SPEC.SY HOME OVERRUN	The specimen syringe motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4016	SPEC.SY ACCELL	The acceleration/deceleration table of specimen syringe motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4017	SPEC.SY CLOG DETECTED	Specimen clog was detected.	The item is not assayed. Repeat assay.
4018	SPEC.Z-AXIS HOME SENSOR	The specimen Z-axis motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4019	SPEC.Z-AXIS HOME NOT FOUND	The home position of the specimen Z-axis motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4020	SPEC.Z-AXIS HOME OVERRUN	The specimen Z-axis motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4022	SPEC.Z-AXIS ACCELL	The acceleration/deceleration table of the specimen Z-axis motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4023	SPEC.R-AXIS HOME SENSOR	The specimen R-axis motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4024	SPEC.R-AXIS HOME NOT FOUND	The home position of the specimen R-axis motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4025	SPEC.R-AXIS HOME OVERRUN	The specimen R-axis motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4027	SPEC.R-AXIS ACCELL	The acceleration/deceleration table of the specimen R-axis motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

7.1. List of Error Messages

Actuator-related errors

No.	Error message	Description	Troubleshooting
4028	SPEC.T-AXIS HOME SENSOR	The specimen θ -axis motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4029	SPEC.T-AXIS HOME NOT FOUND	The home position of the specimen θ -axis motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4030	SPEC.T-AXIS HOME OVERRUN	The specimen θ -axis motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4032	SPEC.T-AXIS ACCELL	The acceleration/deceleration table of the specimen θ -axis motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4033	SEAL BREAK HOME SENSOR	The seal breaker motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4034	SEAL BREAK HOME NOT FOUND	The home position of the seal breaker motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4035	SEAL BREAK HOME OVERRUN	The seal breaker motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4037	SEAL BREAK ACCELL	The acceleration/deceleration table of the seal breaker motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4038	WASH.PROBE HOME SENSOR	The BF probe motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4039	WASH.PROBE HOME NOT FOUND	The home position of the BF probe motor cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4040	WASH.PROBE HOME OVERRUN	The BF probe motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4042	WASH.PROBE ACCELL	The acceleration/deceleration table of the BF probe motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4043	WASH.SY HOME SENSOR	The BF syringe motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4044	WASH.SY HOME NOT FOUND	The BF syringe motor home position cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4045	WASH.SY HOME OVERRUN	The BF syringe motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4047	WASH.SY ACCELL	The acceleration/deceleration table of the BF syringe motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4048	SUBST.SY HOME SENSOR	The substrate syringe motor home sensor remains activated.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

7.1. List of Error Messages

Actuator-related errors

No.	Error message	Description	Troubleshooting
4049	SUBST.SY HOME NOT FOUND	The substrate syringe motor home position cannot be detected.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4050	SUBST.SY HOME OVERRUN	The substrate syringe motor overran on the home side.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4052	SUBST.SY ACCELL	The acceleration/deceleration table of the substrate syringe motor was incorrectly set.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
4053	SEAL BREAK POS. SENSOR	The seal breaking position sensor is faulty.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

System-related errors

No.	Error message	Description	Troubleshooting
5001	INTERNAL ERROR	Internal program error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5002	NO RESPONSE FROM SLAVE	Slave response not detected error	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5003	SLAVE COMMAND ERROR	Slave command error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5004	SLAVE FIFO ERROR	Slave FIFO error	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5005	MAIN PROGRAM ERASE TIMED OUT	Main program erase timeout.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5006	MAIN PROGRAM WRITE ERROR	Main program write error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5007	MAIN PROGRAM COMPARE ERROR	Main program compare error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5008	MAIN PROGRAM NOT INSTALLED	Main program not found.	Contact the local Tosoh representative.
5009	SLAVE PROGRAM ERASE TIMED OUT	Slave program erase timeout.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5010	SLAVE PROGRAM WRITE ERROR	Slave program write error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5011	SLAVE PROGRAM COMPARE ERROR	Slave program compare error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5012	SLAVE PROGRAM NOT INSTALLED	Slave program not found.	Contact the local Tosoh representative.
5013	INSTALLATION ERASE TIMED OUT	Image data erase timeout.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

7.1. List of Error Messages

System-related errors

No.	Error message	Description	Troubleshooting
5014	INSTALLATION WRITE ERROR	Image data write error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5015	INSTALLATION COMPARE ERROR	Image data compare error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5016	INSTALLATION NOT INSTALLED	Image data not found.	Contact the local Tosoh representative.
5017	PRINTER HARD ERROR	Printer hardware error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5018	ASSAY ABORTED	Measurement terminated.	Repeat assay.
5019	DETECTOR CALIB. ABORTED	Detector calibration aborted	Check the conditions, Repeat the detector calibration.
5020	DETECTOR TASK ERROR	Detector calibration task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5021	TURNTABLE TASK ERROR	Turntable task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5022	SPECIMEN TASK ERROR	Specimen arm task execution error.	Turn the power off and on again. Send the printed error report to the local Tosoh representative.
5023	SEAL BREAK TASK ERROR	Seal break task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5024	CCD TASK ERROR	Cup read task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5025	SUBSTRATE TASK ERROR	Substrate task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5026	WASHER TASK ERROR	BF washing task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5027	DRAIN TASK ERROR	Drain task execution error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5029	CSUM ERROR (PARAM)	Control parameter checksum error.	Turn the power off and on again and check the parameters. If this problem reoccurs, contact the local Tosoh representative.
5030	CSUM ERROR (REAGENT)	Test file checksum error.	Turn the power off and on again and check the test file and calibration curve. If this problem reoccurs, contact the local Tosoh representative.
5031	CSUM ERROR (RESULT)	Assay result checksum error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.

7.1. List of Error Messages

System-related errors

No.	Error message	Description	Troubleshooting
5032	CSUM ERROR (ERRLOG)	Error log checksum error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5033	CSUM ERROR (OPERATION LIST)	Operation log checksum error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5034	TESTFILE FLASH COMPARE ERROR	Test file data write compare error.	Turn the power off and on again. If this problem reoccurs, contact the local Tosoh representative.
5035	MUTEX LOCK UNLOCK ERROR	Control variable acquisition error for sample dispensing task.	Send the printed error report to the local Tosoh representative.

7.2. List of Flags

A flag is attached to an assay result as appropriate: an error flag if an assay does not complete normally because of a problem or a user flag (normal or abnormal value) to enable the user to discriminate an assay result.

When an error flag is attached, the assay result may or may not be available depending on the error. When an error flag is not attached, the result of a normally finished assay is available. If no assay result is available due to an error, take the appropriate action according to **Section 7.2.1 “Flag Lists”** and **Section 7.2.2 “Detailed Meanings of Flags and Action”**.

7.2.1. Flag lists

Error flags

FLAG	Meaning	Action	CAL.	Result
SE	System error	Terminate assay	REJECT	INCOMPLETE
ME	Item error (unable to assay)	Do not assay	REJECT	INCOMPLETE
AE	Test cup read error	Do not assay	REJECT	INCOMPLETE
NB	Seal breaking failure	Do not assay	REJECT	INCOMPLETE
IM	Sample ID mismatch	Do not assay	REJECT	INCOMPLETE
WU	B/F washing failure	Do not assay	REJECT	INCOMPLETE
DS	Insufficient diluent	Do not assay	REJECT	INCOMPLETE
WS	Insufficient wash solution	Do not assay	REJECT	INCOMPLETE
SS	Insufficient sample	Do not assay	REJECT	INCOMPLETE
SP	Waste liquid full	Do not assay	REJECT	INCOMPLETE
SC	Nozzle clogged	Do not assay	REJECT	INCOMPLETE
LE	Lot read error	Do not assay	REJECT	INCOMPLETE
DO	Over detector range	Perform assay	REJECT	INCOMPLETE
NC	No calibration curve	Perform assay	-	RATE
CE	Operation error	Perform assay	REJECT	INCOMPLETE
<L	Lower than the calibration area	Perform assay	-	RATE
>H	Higher than the calibration area	Perform assay	-	RATE
IO	Imperfect temperature control	Perform assay	REJECT	RATE
MF	Mechanical error in dispensing sample	Do not assay	REJECT	INCOMPLETE
BS	Insufficient enzyme substrate	Perform assay	REJECT	INCOMPLETE
HB	High substrate blank	Perform assay	REJECT	RATE
CV	Calibration curve expired If 60 days or more pass after the expiry date, assay results will be reported in rate values with NC flags.	Perform assay	-	CONC
DL	Insufficient substrate dispensing volume or low detector light intensity	Perform assay	REJECT	RATE
MA	Mismatch between reading and order (CALIBRATION)	Use reader Info	REJECT	-

7.2. List of Flags

User flags

L	Lower than (user) reference range	Perform assay	-	CONC
H	Higher than (user) reference range	Perform assay	-	CONC
	No flag indicates normal result	Perform assay	ACCEPT	CONC

Abbreviations

CAL.	ACCEPT	Calibrator data automatically accepted
	REJECT	Calibrator data automatically rejected
Result	INCOMPLETE	Assay result incomplete
	RATE	Only rate value obtained
	CONC	Rate and concentration value obtained

7.2.2. Detailed Descriptions of Flags and Actions

SE: The assay could not be completed due to a problem (error) that does not disable the device.

ME: The assay item could not be read at calibration or it was an item which cannot be used in AIA-360. Check labelling on the test cup and repeat assay.
If this flag appears continuously, the cup reader may have been displaced.
Contact the local Tosoh representative.

Point

This flag may be attached if the test cup is not checked by pressing [] in the CALIB REQUEST (Check START) screen.

AE: The assay item could not be read by the cup reader.
In this case, no assay request is assumed and the assay is cancelled. Check labelling on the test cup and repeat assay.
If this flag appears continuously, the cup reader may have been displaced.
Contact the local Tosoh representative.


NB: The seal of the test cup could not be broken. The assay is cancelled.
The seal breaker may have a dirty blade or be displaced.
Contact the local Tosoh representative.

7.2. List of Flags

- IM: The sample was skipped because the input sample ID did not match the one read by the built-in barcode reader. Repeat assay after checking the barcode label position and quality and also the sample order.
- WU: During B/F washing, the wash solution could not be drained.
If this flag appears continuously, the tip of the B/F washing probe may be dirty or clogged. Contact the local Tosoh representative.
- DS: Insufficient diluent has been detected. Replenish the diluent and repeat assay.
- WS: Insufficient wash solution has been detected. Replenish the wash solution and repeat assay.
- SS: The assay was cancelled because of insufficient sample. If this flag appears when there is an enough sample, either the sample nozzle or the sample detection sensor may be faulty. If this problem occurs frequently, contact the local Tosoh representative.
- SP: The waste bottle has become full. Discard the waste liquid and repeat assay.
- SC: Dispensing was cancelled because clogging was detected during sample suction. Check that the sample is free of fibrin or other substances. **If the sample is not clotted, the sample nozzle may be faulty or the tubing may be blocked.** If this problem occurs frequently, contact the local Tosoh representative.
- LE: The lot number of the assay item could not be read by the cup reader. In this case, no assay request is assumed and the assay is cancelled. Check labelling on the test cup and repeat assay.
If this flag appears continuously, the cup reader may have been displaced. Contact the local Tosoh representative.
- DO: No result could be obtained because the measuring range of the detector was exceeded. Dilute the sample as required and repeat assay.

7.2. List of Flags

- NC: No result was obtained because there was no calibration curve for the item or lot.
Alternatively, the concentration could not be calculated because the calibration curve has expired 60 days ago or earlier.
In these cases, create a calibration curve and recalculate to obtain a result.
- CE: No result was obtained because an operation error occurred during the rate calculation or the conversion of concentration. An item using a multi-point calibration curve may result in an error for some relationship between the shape of the calibration curve and the conversion range of concentration. Check that the calibration curve does not have the minimum value or the maximum value in the calibration area (see the figure) and that the calibration area is in the range specified by the manufacturer.
For the range of calibration area, the minimum value is set to ASSAY L and the maximum value to ASSAY H in the TEST FILE screen.

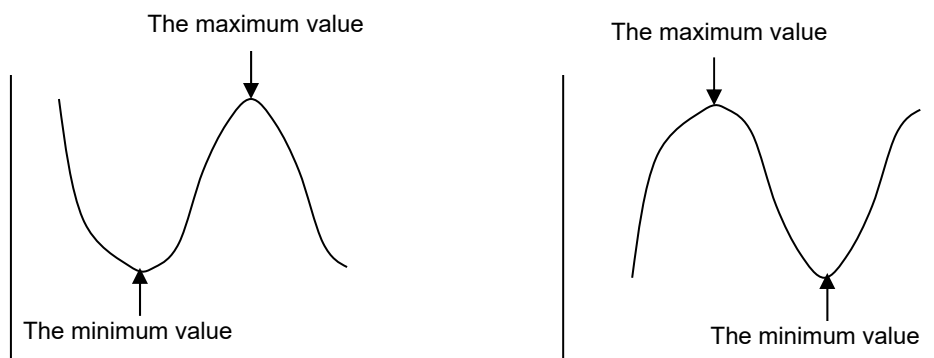

- <L: The assay result was not accepted because it lies below the calibration area.
- >H: The assay result was not accepted because it lies above the calibration area.
Dilute the sample as required and assay it again.
- IO: The temperature exceeded the controllable range.
If this flag appears frequently, contact the local Tosoh representative.

7.2. List of Flags

- MF: A flag is attached due to an abnormality occurring during sample dispensing. Operation continues but a return failure disables the assay.
- BS: There is insufficient enzyme substrate.
Replace the enzyme substrate.
- HB: The substrate has decomposed and the blank is high. If the substrate blank is high, dispersion in a low enzyme activity area will be large. Replace the substrate and repeat assay. If the HB flag appears even after the substrate is replaced, the substrate line may be contaminated. In this case, contact the local Tosoh representative.
- CV: The calibration curve has expired.
Set up the calibration curve for the same lot and recalculate in the RESULT REVIEW screen.
If 60 days or more pass after the expiry date, assay results will be reported in rate values with NC flags.
- DL: The substrate dispensing amount is less than the specified amount or the lamp intensity of the fluorescence detector is low. If the DL flag is attached, replace the substrate (MAINT screen → 6. REPLACE SUBSTRATE ) and repeat assay. If the DL flag appears again, contact the local Tosoh representative.
- MA: The assay item read by the camera is different from the requested assay item. Check the read and requested items.

Point

This flag may be attached if the test cup is not checked by pressing  in the CALIB REQUEST (Check START) screen.

7.2. List of Flags

7.2.3. Meanings of Daily Check Flags and Actions

After performing a daily check on the substrate background, the result is printed. The printed flags have the following meanings:

(1) Substrate Replacement

OK: Liquid substitution with the enzyme substrate is sufficient.

ERR: Liquid substitution with the enzyme substrate is insufficient or the detector lamp intensity decreased. Check the remaining amount of enzyme substrate and perform the daily check again.

If an 'ERR' appears again, please contact your Tosoh local representative.

(2) 4MU Background

OK: The fluorescence intensity (background intensity) of the enzyme substrate is below 1500 nmol/L.

HB: The fluorescence intensity (background intensity) of the enzyme substrate is 1500 nmol/L or more. Replace the enzyme substrate and perform daily check again.

(3) Lamp Intensity Level


OK: The lamp intensity of the detector is sufficient.

LL: The lamp doesn't light or the lamp intensity of the detector is not sufficient. Please contact your Tosoh local representative..

NOTES

Chapter 8: Shut Down Operation (Shut Down Menu)

8.0.Introduction

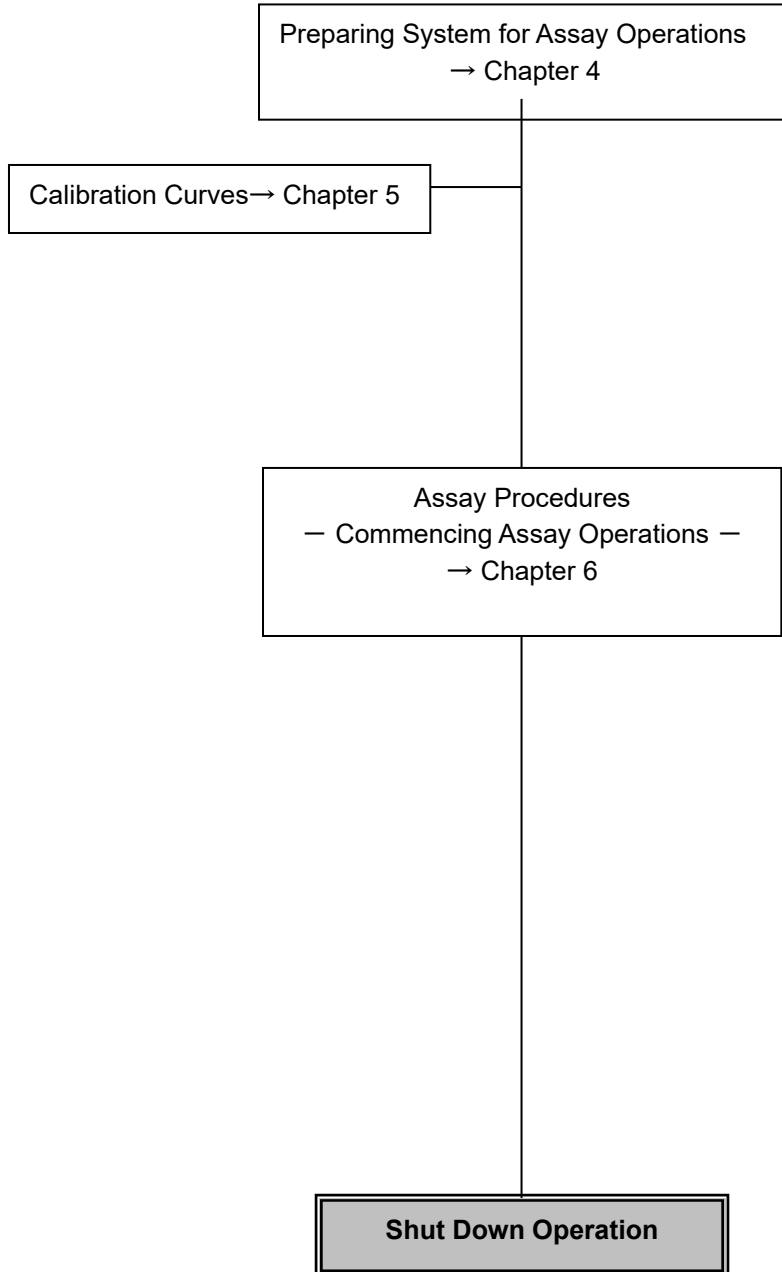

8.1. Shut Down Operation (Shut Down Menu)

Make sure to prime the substrate lines at the end of each day of operation. Leaving the substrate in the lines will result in fluid evaporation and precipitation of the reagent, which may clog the lines. Residual substrate in the lines may also cause a higher background measurement.



Replace the substrate in the lines by priming them with 70% ethanol or 70% isopropyl alcohol solution.

Also note that priming the lines with distilled water will contaminate the lines and cause higher background measurement results for the enzyme substrate.

Procedures


- (1) Remove all sample cups, test tubes and reagent cups for which assays have been completed.
- (2) Remove the enzyme substrate bottle and replace it with 70% ethanol or 70% isopropyl alcohol bottle.



- Seal the enzyme substrate bottle with a clean rubber stopper or parafilm and place in refrigerator.
- Diluent and wash solution do not require refrigeration, so do not need to be removed.

- (3) Press **MENU** to display the MENU screen.

- (4) Press .

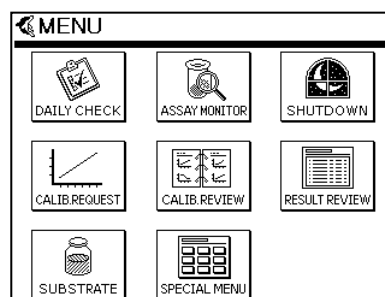


<MENU Screen>

- (5) Message on the SHUT DOWN screen. This displays "Set substrate replacement solution and press START".

Point

Note that the SHUT DOWN screen is not displayed during the assay operations

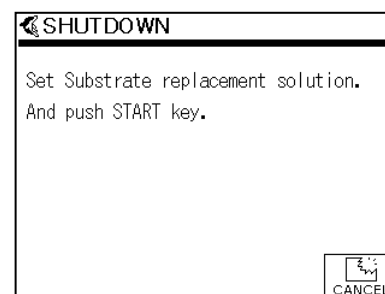


<SHUT DOWN Screen>

8.1. Shut Down Operation (Shut Down Menu)


- (6) Press **START** to commence the substrate replacement operation.
The “Please Wait...” message is displayed while the priming operation is in progress.



A shut down operation in progress can be terminated by pressing .

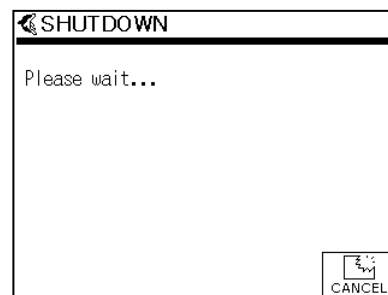

- (7) “Please Turn off the Power” will appear on the screen, indicating that the priming operation is complete.
Turn off the system power supply.

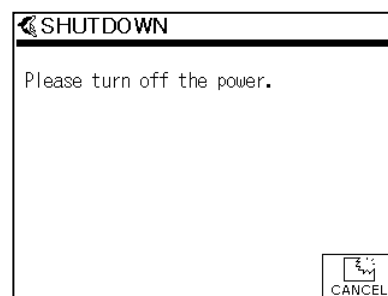

Point


Note that assay results are retained in the system memory after the power is turned off. System memory is capable of storing up to 800 assay results. Assay results are deleted in order starting from the oldest as new results are entered in the memory.


NOTES

Chapter 9: Other Functions in SPECIAL MENU

The SPECIAL MENU provides the menus required for entering various system operation settings and maintenance utility functions.

Press  in the MENU screen to display the SPECIAL MENU screen.

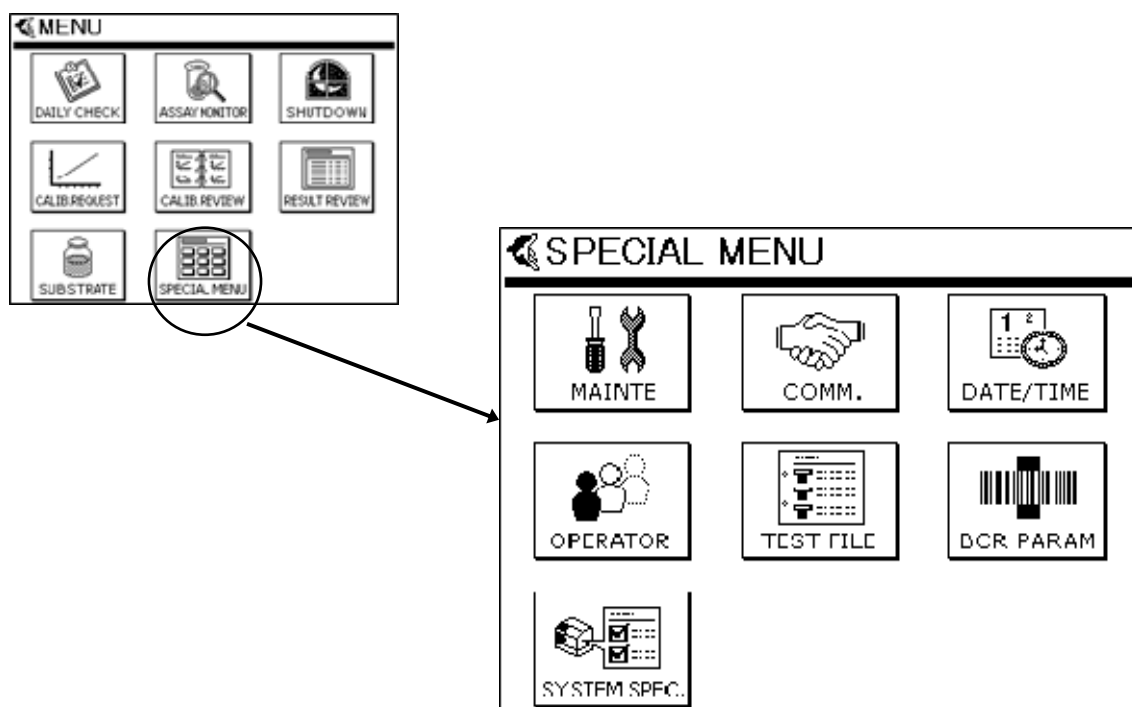



	MAINT	Used to monitor the status of various system components.
	COMM.	RS232C transmission parameter settings
	DATE/TIME	Used to set date and time.
	OPERATOR	Used to register and change operator names.
	TEST FILE	Used to enter parameters for individual test items (analytes).
	BCR PARAM	Used to enter barcode parameters.
	SYSTEM SPEC.	Used to enter system operating specifications.

9.1.MAINT (Maintenance Tool)

This utility is used to check the operating status of the AIA-360 system's various operating components.


Basic Operating Procedures

- (1) Go to MAINT SCREEN, move cursor to the item to be checked and press .

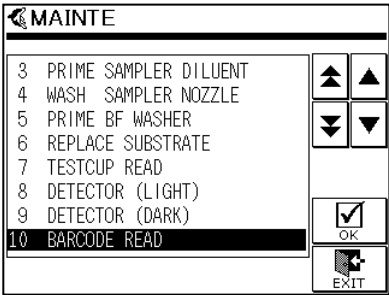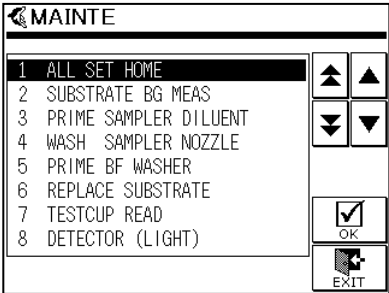

<MAINT Screen>

- (2) The WAIT screen (Please Wait...) appears while the selected item is being checked.

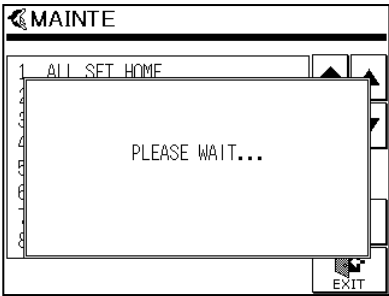

<WAIT Screen>

- (3) The status check is completed by pressing  when "Complete!" appears on the screen.



<Complete! Screen (Sample)>



Please observe the operation checking procedures whenever they are provided for specific items.

9.1 MAINT (Maintenance Tool)

1: ALL SET HOME : Moves the various system components back to their correct start positions.

2: SUBSTRATE BG MEAS : Performs substrate background measurement.



Perform after installing a new substrate solution bottle, but first use “6:REPLACE SUBSTRATE” to prime the enzyme substrate lines.

- (1) Place 1 detector standardization test cup (STD cup) in the No. 1 position (slot) in the reagent cup holder.
- (2) Move cursor to “2:SUBSTRATE BG MEAS.”
- (3) Press the  button to activate the carousel and perform substrate background measurement.
- (4) The “Complete! Screen” is displayed and measured results are printed out when the measuring operation completes.

Fig 9-1 Sample Printout of Substrate Background Measurement Results

```

***SUBSTRATE BACKGROUND ***
OP:      10/07/01 13:28

Date      : 10/07/01 13:28
SubstrateReplacement:OK
4MU Background :OK
bG
LampIntensity Level :OK
BG Smp      :990
BG Ref      :1352
Subst Smp   :2113
Subst Ref   :25236
***END***
  
```

Arrows point from the following numbers to the corresponding lines in the printout:

- 1** points to SubstrateReplacement:OK
- 2** points to 4MU Background :OK
- 4** points to bG
- 3** points to LampIntensity Level :OK

1. Indicates whether substrate replacement using the new substrate solution was successful.
 OK: When successful
 ERR: When unsuccessful
2. Indicates whether the operation to measure fluorescent intensity (background intensity) of the enzyme substrate detected any problems. This is reported with value in nmol/L.
 OK: When lower than 1500 nmol/L (No problem)
 Hb: When equal to or higher than 1500 nmol/L (Background was too high)
3. Indicates the status of detector lamp intensity.
 OK: When sufficient
 LL: When insufficient → Contact a Local Tosoh representative
4. Measurement value

9.1. MAINT (Maintenance Tool)

3: PRIME SAMPLER DILUENT : Used when filling up diluent

This is used when priming system with diluent.

(1) Prime the system with diluent.

(2) Move cursor to “3:PRIME SAMPLER DILUENT” and press



This launches the diluent filling operation.

4: WASH SAMPLER NOZZLE : Used for washing sampling nozzle

5: PRIME BF WASH

: Used when filling wash solution.

This is used when priming system with wash solution.

(1) Prime the system with wash.

(2) Move cursor to “5:PRIME BF WASH” and press



to start the filling operation.

6: REPLACE SUBSTRATE : Used when priming enzyme substrate lines

This is used when priming system with new substrate.

(1) Replace current substrate with a new bottle of substrate.

(2) Move cursor to “6:REPLACE SUBSTRATE” and press



to start the substrate priming operation.



When substrate priming is finished, use “2:SUBSTRATE BG MEAS” to perform substrate background measurement.

7: TESTCUP READ : Used when performing reagent cup read test

(1) Use the **SAMPLE FEED** key to move the cup reader into position when performing a read test on a reagent cup.

(2) Move cursor to “7:TESTCUP READ” and press



This reads the reagent cup analyte code and lot number located below the cup reader and displays them on the screen.

9.1. MAINT (Maintenance Tool)

8: DETECTOR (LIGHT) : Used for Testing Fluorescent Detector

- (1) Use the **SAMPLE FEED** key to move the reagent cup to a position below the fluorescent detector unit.

- (2) Move cursor to "8:DETECTOR (LIGHT) and press . This displays detector data. (While lamp is on.)

9: DETECTOR (DARK) : Used to Test Fluorescent Detector Unit (Dark measurement)

- (1) Use the **SAMPLE FEED** key to move the reagent cup to be tested to a position below the fluorescent detector unit.

- (2) Move cursor to "9:DETECTOR (DARK) and press . This displays detector data. (While lamp is off.)

10: BARCODE READ : Used to Test Barcode Read Performance

- (1) Use the **SAMPLE FEED** key to move the primary tube to be read beside the barcode reader.

- (2) Move cursor to "10:BARCODE READ" and press . This performs the barcode read operation and displays the data.

9.2. Communications (RS232C Transmission Parameter Settings)

The AIA-360 uses the RS232C serial interface for transmitting data with external devices. Enter the parameter settings required for transmitting with the selected external device. The settings in parentheses to the right are the ones currently selected for that parameter.

Move cursor to the desired parameter and press



to select.

COMM.	
1:PROTOCOL	(TRANSPARENT)
2:DATA LENGTH	(8 BIT)
3:PARITY CHECK	(NONE)
4:STOP BIT LENGTH	(1)
5:BAUD RATE	(19200)

▲

▼

PRINT

MODIFY

EXIT

<COMM. Screen>

These settings must be entered or updated the first time the AIA-360 is started or when changes to the settings are required. Note that the new settings are stored in the system memory and retained, even when the power is turned off.

For detailed descriptions of transmission protocols and hardware settings, refer to "Appendix B: RS232C Transmission" in "Chapter 12."



Note that transmission settings cannot be modified while assay operations are in progress.



Pressing  will print out the current screen.

Fig. 9-2 Sample print out of transmission parameters


```

***  COMM      PARAMETER  ***
OP:N0.002      04/01/09 15:49

1:PROTOCOL      (TRANSPARENT)
2:DATA LENGTH   (8 BIT)
3:PARITY CHECK   (NONE)
4:STOP BIT LENGTH ( 1 )
5:BAUD RATE     (19200)
***END***
  
```

9.3.DATE/TIME (Time and Date Settings)

- (1) Press  to display the DATE/TIME screen.

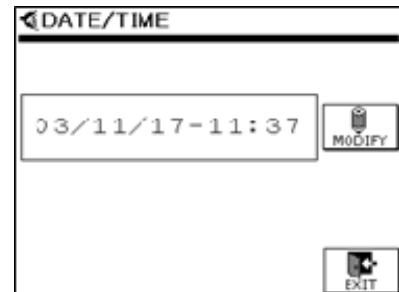


<DATE/TIME Screen>

- (2) Press  to display the DATE/TIME INPUT screen.

- (3) Enter the current time and date then press



to redisplay the DATE/TIME screen.

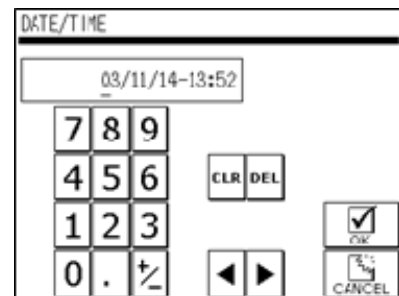

<DATE/TIME INPUT Screen>

9.4.OPERATOR (Registering and Changing)

The OPERATOR screen is used to register new operators, or change or delete currently registered operators.


For a detailed description, refer to section “2.1 Confirming/Selecting Operator Name) in “Chapter 4.”



The operator name is included on system printouts.

9.5. TEST FILE (of Analyte parameters)

The AIA-360 enables users to check and modify certain parameter settings for the individual analytes used in the assaying of reagents. Users are able to select the reference range and decimal place settings for parameters as necessary.

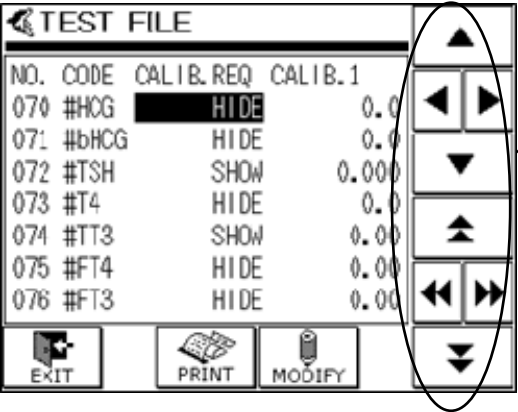

The TEST FILE consists of multiple pages, which can be scrolled through using the arrow keys.



- TEST FILE settings cannot be modified while assay operations are in progress.
- Note that the new settings are stored in the system memory and retained even when the power is turned off.
- Changes made to parameter settings will be saved when the operator leaves the TEST FILE screen to go to another screen. It is important to note that parameter changes will be lost if system power is lost while still in the TEST FILE screen.



Parameter information can be printed by pressing .

Fig. 9-3 Sample TEST FILE Printout

```
*** TEST FILE REPORT ***
OP:NO.002   04/01/09 16:02

Code       :004
Analyte    :BMG
Unit       :mg/l
Decimal    :4
Specimen Vol.:15
Diluent Vol.:135
Reference(L):0.0020
Reference(H):0.4000
Assay (L) :0.0020
Assay (H) :0.4000
Factor1 (A):1.000000
Factor1 (B):0.000000
Factor2 (A):1.000000
Factor2 (B):0.000000
Calib Code :4
Calib Reps :3
Calib Conc(1):0.00000
Calib Conc(2):0.01250
Calib Conc(3):0.05000
Calib Conc(4):0.15000
Calib Conc(5):0.30000
Calib Conc(6):0.40000
Virtual Conc:0.00000
Graph Origin:0.00000

***END***
```

9.5. TEST FILE (of Analyte parameters)

Column Name	Description	
NO.	Analyte code	Number from 0 to 127 unique to each analyte.
CODE	Analyte name	Abbreviated name consisting of five alphanumerics.
CALIB.REQ*	Specifies whether this Analyte code is displayed or not on the screen.	
CALIB.1 to 6	Calibration concentrations	
CAL LOT L CAL LOT R	Number of the lot for which calibration curves were selected. The AIA-360 allows for the creation of 2 lots of calibration curves per analyte. Lot numbers for current calibration curves are displayed under LOT. L and LOT. R.	
UNIT	Units of concentration	Unit of measurement for concentration.
SMPL. VOL	Sample volume	Sample volume (μl).
DIL. VOL	Diluent volume	Volume of diluent dispensed together with sample (μl).
ASSAY L	Assay range lower limit	Designates minimum effective assay concentration. Concentrations below this limit are not assayable.
ASSAY H	Assay range upper limit	Designates maximum effective assay concentration. Concentrations higher, even if mathematically viable, cannot be used as concentration values.
REF. L*	Reference range lower limit	Users can specify as required.
REF. H*	Reference range upper limit	Users can specify as required.
DECIMAL*	Decimal places	Designates the effective number of decimal places for expressing concentrations. Users can specify as required.

Procedures for Setting CALIB.REQ* Places

- <1> Move cursor to "CALIB REQ*" column and press .
- <2> Select "SHOW" and "HIDE".
- SHOW : Display
- HIDE : Do not display

Procedures for Setting REF. L*, REF. H* and DECIMAL* Places

- <1> Move cursor to desired column and press .
- <2> Enter desired values when the INPUT screen is displayed.
- <3> Press  to confirm setting.



Note that users cannot change settings other than those for CALIB REQ*, REF. L*, REF. H* and DECIMAL* Places.

9.6. BCR PARAM (Detailed Barcode Settings)

These settings are used to specify various barcode parameters.

The settings in parentheses to the right are the ones currently selected for that parameter.

To change the setting, move the cursor to the design parameter and press  to change a value or a enter setting.

1: BCR START DIGIT

Designates start digits (1 to 15) for reading the barcode IDs attached to specimens.

Default: 1

2: BCR LENGTH

Designates the maximum double-digit length (1 to 16) for reading the barcode IDs attached to specimens.

Default: 16

3: CODE39

Specifies whether or not to read the CODE39 barcode label.

Default value: YES (read)

ST/SP CHAR OUTPUT

Designates the start or stop character for reading CODE39 barcode labels.

Default value: OFF (unused)

CHECK DIGIT CHECK


Specifies the check setting for the CODE39 check digit.

Default value: OFF (does not check)


CHECK DIGIT OUTPUT

Specifies whether or not to send check digit for CODE39 barcode label.

Default value ON (used)

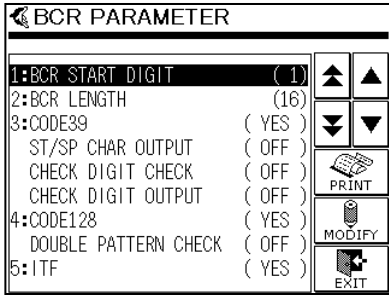

BCR PARAMETER	
1:BCR START DIGIT	(1)
2:BCR LENGTH	(16)
3:CODE39	(YES)
ST/SP CHAR OUTPUT	(OFF)
CHECK DIGIT CHECK	(OFF)
CHECK DIGIT OUTPUT	(OFF)
4:CODE128	(YES)
DOUBLE PATTERN CHECK	(OFF)
5:ITF	(YES)

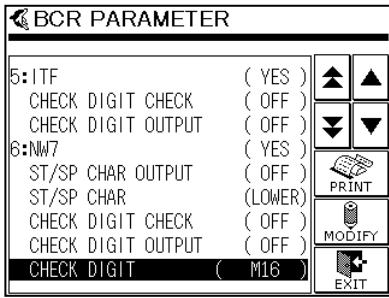

BCR PARAMETER	
5:ITF	(YES)
CHECK DIGIT CHECK	(OFF)
CHECK DIGIT OUTPUT	(OFF)
6:NW7	(YES)
ST/SP CHAR OUTPUT	(OFF)
ST/SP CHAR	(LOWER)
CHECK DIGIT CHECK	(OFF)
CHECK DIGIT OUTPUT	(OFF)
CHECK DIGIT	(M16)

<BCR PARAMETER Screen>



- When CHECK DIGIT CHECK is set to OFF, CHECK DIGIT OUTPUT automatically becomes ON and cannot be switched to OFF.
- When CHECK DIGIT CHECK is set to OFF, not all digits can be used as an ID without setting CHECK DIGIT OUTPUT to ON.

9.6. BCR PARAM (Detailed Barcode Settings)

4: CODE128

Specifies whether or not to read the CODE128 barcode label.

Default value: YES (read)

DOUBLE PATTERN CHECK

Specifies whether or not to use double character start pattern for CODE39 barcode label.

Default value: OFF (unused)

5: ITF

Specifies whether or not to read the ITF barcode label.

Default value: YES (read)

CHECK DIGIT CHECK

Specifies the checks setting for the ITF check digit.

Default value: OFF (do not check)

CHECK DIGIT OUTPUT

Specifies whether or not to send check digit for ITF barcode label.

Default value: ON (used)

BCR PARAMETER	
5:ITF	(YES)
CHECK DIGIT CHECK	(OFF)
CHECK DIGIT OUTPUT	(OFF)
6:NW7	(YES)
ST/SP CHAR OUTPUT	(OFF)
ST/SP CHAR	(LOWER)
CHECK DIGIT CHECK	(OFF)
CHECK DIGIT OUTPUT	(OFF)
CHECK DIGIT	(M16)

Navigation buttons: UP, DOWN, LEFT, RIGHT, PRINT, MODIFY, EXIT.

<BCR PARAMETER Screen>



- When CHECK DIGIT CHECK is set to OFF, CHECK DIGIT OUTPUT automatically becomes ON and cannot be switched to OFF.
- When CHECK DIGIT CHECK is set to OFF, not all digits can be used as an ID without setting CHECK DIGIT OUTPUT to ON.

6: NW7

Specifies whether or not to read the NW7 barcode label.

Default value: YES (read)

ST/SP CHAR OUTPUT

Designates the start or stop character for reading NW7 barcode labels.

Default value: OFF (unused)

ST/SP CHAR

Designates the type of start or stop character for the NW7 barcode label.

Default value: LOWER (lowercase)

CHECK DIGIT CHECK

Specifies the check setting for the NW7 check digit.

Default value: OFF (does not check)

9.6. BCR PARAM (Detailed Barcode Settings)

CHECK DIGIT OUTPUT

Specifies whether or not to send check digit for NW7 barcode label.

Default value: ON (used)



- When CHECK DIGIT CHECK is set to OFF, CHECK DIGIT OUTPUT automatically becomes ON and cannot be switched to OFF.
- When CHECK DIGIT CHECK is set to OFF, not all digits can be used as an ID without setting CHECK DIGIT OUTPUT to ON.

CHECK DIGIT

Designates the type of check digit for the NW7 barcode label.

7 CHK-DR	: 7 check DR
M16	: modulus 16 (Default value)
M11	: modulus 11
M10/2W	: modulus 10/2 wait
M10/3W	: modulus 10/3 wait
M11-A	: weighted modulus 11
M10/2W-A	: runs



BCR PARAM settings cannot be changed while assay operations are in progress. Changes made to parameter settings will be saved when the operator leaves the BCR PARAM screen to go to another screen. Parameter changes are saved in system memory, and thus do not have to be re-entered each time the system is restarted.

Point

Parameter information can be printed by pressing



Fig. 9-4 Sample Barcode Parameter Printout

```

*** BCR      PARAMETER ***
CP:NO.002    04/01/09 16:14

1:BCR START DIGIT      ( 1 )
2:BCR LENGTH           (16)
3:CODE39               ( YES )
  ST/SP CHAR OUTPUT ( OFF )
  CHECK DIGIT CHECK ( OFF )
  CHECK DIGIT OUTPUT( OFF )
4:CODE128              ( YES )
  DOUBLE PTN CHECK  ( OFF )
5:ITF                  ( YES )
  CHECK DIGIT CHECK ( OFF )
  CHECK DIGIT OUTPUT( OFF )
6:NW7                  ( YES )
  ST/SP CHAR OUTPUT ( OFF )
  ST/SP CHAR         (LOWER)
  CHECK DIGIT CHECK ( OFF )
  CHECK DIGIT OUTPUT( OFF )
  CHECK DIGIT        (  M16 )
                        ***END***
  
```

9.7.SYSTEM SPEC. (System Operation Settings)

The various operating conditions for the AIA-360 are entered from this screen.


The settings in parentheses to the right are the ones currently selected for that parameter.

To change setting, move cursor to design parameter and press  to change value or enter setting.

1: REALTIME PRINT OUT

Specifies whether or not to print assay reports for each assay operation.

The factory default is "Yes."

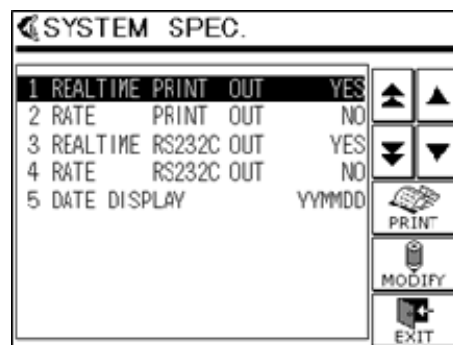

<SYSTEM SPEC Screen>

2: RATE PRINT OUT

Specifies whether or not to output rate when printing assay reports.

The factory default is "No."

3: REALTIME RS232C OUT

Specifies whether or not to output assay reports via the RS232C port for each assay operation.

The factory default is "No."

4: RATE RS232C OUT

Specifies whether or not to output rate when outputting assay reports via the RS232C port.

The factory default is "No."

5: DATE DISPLAY

Specifies the format for displaying the date.

① YY/MM/DD

② MM/DD/YY

③ DD/MM/YY

The factory default is ①.

NOTES

Chapter 10: Maintenance Procedures

This chapter describes the daily inspection and maintenance procedures that users must perform in order to maintain the peak performance capability of AIA-360.


10.1. Daily Maintenance Procedures

10.1.1. System Start-up

For the description of system start-up maintenance procedures, refer to section “2. System Start-up” in “Chapter 4: Preparing System for Assay Operation.”

10.1.2. System Shutdown

For description of system shutdown maintenance procedures, refer to section “1. System Shutdown (Shutdown menu)” in “Chapter 8: Terminating Assay Operations.”



When shutting down the system the enzyme substrate solution in the mobile phase lines must be replaced with a 70 % ethanol or 70% isopropyl alcohol solution. If mobile phase is not washed out with 70% ethanol or 70% isopropyl alcohol, the water content in the mobile phase will evaporate and the reagent/additive will precipitate and clog the lines.



Seal the substrate bottle with a clean rubber stopper or parafilm and refrigerate.

10.2. Weekly Maintenance Procedures

10.2.1. Substrate Line

If the substrate line is dirty, the substrate blank becomes higher. After assays, wash the substrate line following the procedures below every week.

- (1) Replace the substrate bottle with a bottle of 70% ethanol or 70% isopropyl alcohol.
- (2) Prime the substrate line by performing ‘6: REPLACE SUBSTRATE’ on the MAINTENANCE screen.
- (3) Perform step (2) a total of three times.

10.3. Monthly Maintenance Procedures

10.3.1. Updating Calibration Curves

The length of validity of the calibration curve varies according to the item; however, most remain valid for 90 days. Assay results will be flagged with the CV flag when a calibration curve has expired. Update calibration curves as necessary.

10.4. Three-month Maintenance Procedures

10.4.1. Diluent and Wash Solution Bottles

Make sure to clean the diluent and wash solution bottles with aqueous hypochlorite on a regular basis by following the procedures below.

- (1) Discard the solution out of the bottles and rinse them with tap water.
- (2) Pour about 300 ml of tap water and about 3 ml of aqueous hypochlorite into each bottle.
- (3) Tightly cap the bottles and wash them by rigorously shaking them. If the bottle is very dirty, leave it for an hour.
- (4) Rinse them thoroughly under running water not to leave hypochlorous acid.
- (5) Rinse them in purified water.

If you use extra tanks to reserve diluent or wash solution, wash the extra tanks in the same procedure.

10.5. Six-Month Cycle Maintenance Procedures

10.5.1. Diluent and Wash Lines

It is effective to clean the diluent and wash lines at the same time to clean the diluent and wash solution bottles. Note that it takes an hour.

- (1) Pour about a litre of purified water and 10 ml of aqueous hypochlorite into a clean reservoir.
- (2) Remove the tubes from the diluent and wash solution bottles and detach the filters from the tube ends. Put the tube ends into the reservoir prepared at the procedure 1). The procedures 3) – 6) should be performed as quickly as possible not to expose the metallic sensor portion to aqueous hypochlorite for a long time.
- (3) Perform '**3: PRIME SAMPLER DILUENT**' on the MAINT screen five times to fill the diluent line with aqueous hypochlorite. Next perform '**5: PRIME BF WASHER**' on the same screen five times to fill the wash line with aqueous hypochlorite.
(Even when an error "2015 BF PROBE PURGE FAILURE" occurs, ignore the error and continue the operation.)
- (4) Pour about a litre of purified water into another clean reservoir and put the tube ends into this reservoir. Make sure the metallic sensor portion exposed to aqueous hypochlorite is to be washed well with purified water so as not to leave any residual hypochlorous acid.
- (5) Leave them for about five minutes.
- (6) Perform '**3: PRIME SAMPLER DILUENT**' and '**5: PRIME BF WASHER**' on the MAINT screen five times each to remove hypochlorous acid from the diluent and wash line completely.
(Even when an error "2015 BF PROBE PURGE FAILURE" occurs, ignore the error and continue the operation.)
- (7) Prepare the diluent and wash solution in the cleaned diluent and wash solution bottles respectively. Attach new filters to the diluent and wash line tube ends and put them into each bottle. Be sure not to put the tube ends into the wrong bottles.
- (8) Perform '**3: PRIME SAMPLER DILUENT**' and '**5: PRIME BF WASHER**' five times each.
(Even when an error "2015 BF PROBE PURGE FAILURE" occurs, ignore the error and continue the operation.)

10.5.2. Replacing Filters for Diluent and Wash Solution Bottles






Make a point of replacing the in-line diluent and wash solution bottle filters on a regular basis. Do this by removing the tubes from the diluent and wash solution bottles, detaching the filters from the tube ends and replacing them with new ones. (Part no. 0018585)

10.6. If AIA-360 Becomes Dirty


Wet a cloth with a neutral detergent; wring well, and wipe down the dirty area of the instrument. If the instrument is very dirty, use a cloth wetted with the 70% ethanol or 70% isopropyl alcohol solution. Avoid water or moisture build-up on the surface of the AIA-360 system, as it may cause the metal to rust.

Chapter 11: Consumable Supplies/Optional Parts

11.1. Consumable Supplies

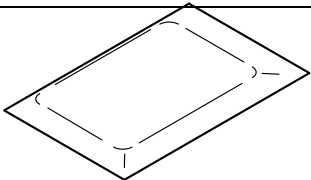Part no.	Part Name and Specifications	Schematic Diagram	No. Included
019510	PRINTER PAPER CORE SHAFT For AIA-360		1
0020107	PROBE TIP		6/pack
0020970	DETECTOR STANDARDIZATION CUP (STD CUP)		200/box
0018581	SAMPLE CUPS		1000/pouch
0019563	PRINTER PAPER 60 mmx42 m		10 rolls/box
0019398	WASTE BOX		1
0018585	TANK FILTERS		10/pouch
0018619	BOTTLE 30 ml		1

11.2. Optional Parts

Part no.	Part Name and Specification	Schematic Diagram	No. Included
0021207	PLUG-2.SUBSTRATE		1




The components of the diluent, wash solution, and waste fluid bottles and the level sensor lead wire are different depending on the date of manufacture. Either sets of parts “before change” or “after change” are provided with the instrument.

Note that the applicable parts cannot be used in combination with the parts “before change” and “after change”.


Before change (plug socket type)

Diluent, Wash solution, waste liquid bottles, and level sensor lead wire

Part no.	Part Name and Specification	Schematic Diagram	No. Included
0021067	DILUENT BOTTLE: with label 500 ml		1
0021068	WASH SOLUTION BOTTLE: with label 1000 ml		1
0021069	WASTE BOTTLE: with label 1000 ml		1
0021138	LEVEL SENSOR LEADS		1

After change (screw type)

Diluent, Wash solution, waste liquid bottles 2 and level sensor lead wire 2

Part no.	Part Name and Specification	Schematic Diagram	No. Included
0024686	Diluent bottle with label 500 ml Part Name: DILUENT BOTTLE-2 WITH LABEL		1
0024687	Wash solution bottle with label 1000 ml Part Name: WASHER BOTTLE-2 WITH LABEL		1
0024687	Waste fluid bottle with label 1000 ml Part Name: WASTE BOTTLE-2 WITH LABEL		1
0024317	Level sensor lead Part Name: LEAD WIRE OF LEVEL SENSOR-2 With screws		1

Chapter 12: Appendix

A. Barcode Label Specifications and Precautions for Use

The following sections outline the specifications for barcode labels used when performing assay operations that utilize the internal barcode reader to read barcode labels applied to primary tubes. Precautions for use are also described.

A.1. Barcode Label Specifications


Applicable barcodes	: CODE128; NW7; CODE39; ITF
Minimum element width	: 0.191 (0.254 or higher recommended) (Narrow width)
PCS	: 0.5 or higher (white reflectance 75%)

A.2. Barcode Effective Read Range

The barcode effective read range is designated as shown below in corresponding to the sample holder slit position.

Point

The barcode reader is unable to read the bottom 20 mm portion. It is important to apply barcode labels near the top of 75 mm primary tubes to ensure effective label reading in cases where sample IDs use a large numbers of digits.

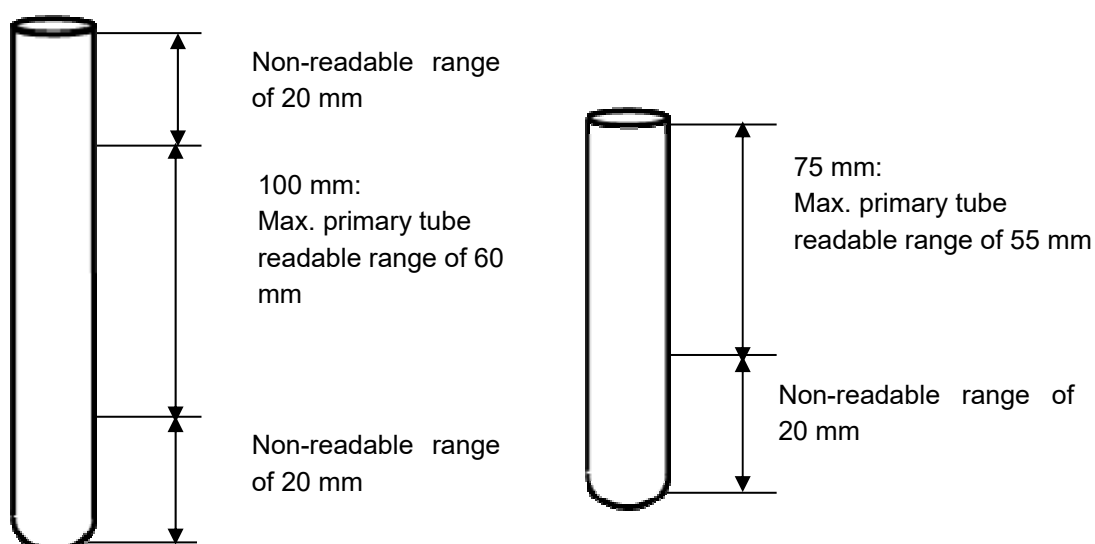

Note: Read range includes barcode margin (quiet zone).

A. Barcode Label Specifications and Precautions for Use

A.3. Maximum Number of Readable Barcode Digits

The table below lists examples of the maximum readable number of barcode digits calculated according to the barcode effective read range.

	Code		Element width (narrow)	Max. no. readable digits	
				75 mm	100 mm
1	CODE128		0.191(min.)	16	16
2			0.254(norm.)		
3	NW7	C/D: no (check digit)	0.191(min.)	16	
4		0.254(norm.)	14		
5		C/D: yes	0.191(min.)	16	
6			0.254(norm.)	13	
7	CODE39	C/D: no	0.191(min.)	16	
8		0.254(norm.)	10		
9		C/D: yes	0.191(min.)	16	
10		0.254(norm.)	9		
11	ITF	C/D: no	0.191(min.)	16	
12		0.254(norm.)			
13		C/D: yes	0.191(min.)		
14		0.254(norm.)			

Note: Calculated with wide: narrow ratio of 2.5 and margin (quiet zone) of 2.54 mm per digit




- Note that the number of readable digits may be limited for CODE39 and NW7, depending on the conditions when using 75 mm test tubes.
- Effective barcode read range may decrease, depending on the quality of the Barcode label used.

A. Barcode Label Specifications and Precautions for Use**A.4. Loading Test Tubes with Barcode Labels**

The sample holders used in the carousel are equipped with slits in order to read the barcodes.

Make sure to position the test tubes with the bar code label facing out of the slit.

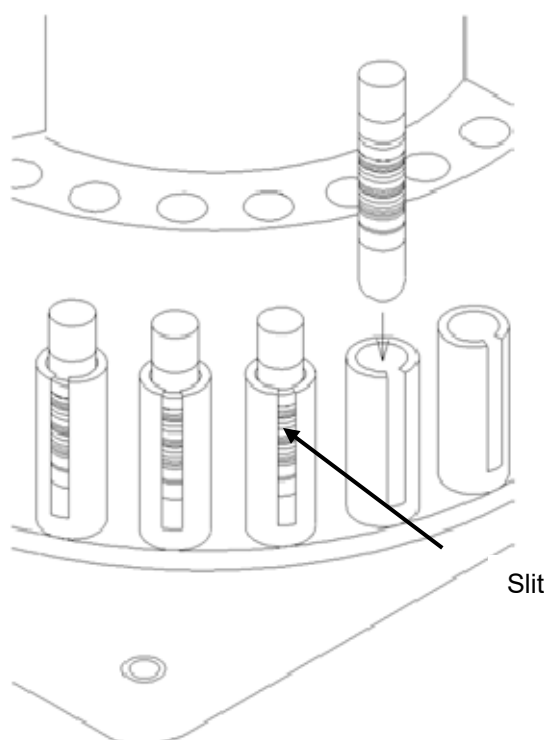

B. RS232C Transmission

The RS232C port provided in the AIA-360 is used for transmitting data to external systems using the following specifications.


B.1. Transmission Specifications

(1) Signal format	RS232C
(2) Transmission format	asynchronous, half duplex
(3) Transmission speed	9600
(4) Data length	8-bit ASCII
(5) Stop bits	1
(6) Parity	NONE
(7) Protocol mode	independent
(8) Check characters	none
(9) Connector	D-SUB(male 9-pin)

B: RS232C Transmission

B.2. Pin Assignment

(1) Standard Configuration

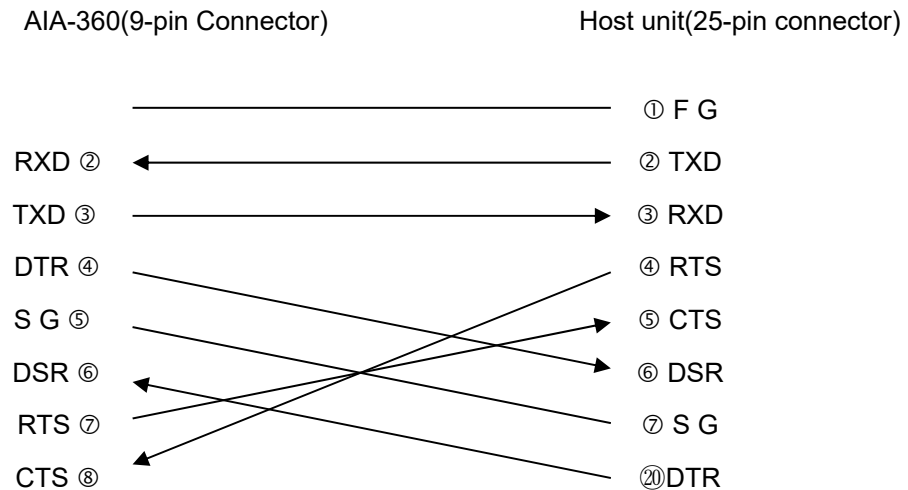

(2) Signal Names

Signal name	Abbreviation	Direction	Description
Frame ground	FG	-	Used to ground frame.
Data send	TXD	output	Sends data from AIA-360. Off when data not present.
Data receive	RXD	input	Receives data coming to AIA-360. Off when data not present.
Request to send	RTS	output	On during request to send.
Clear to send	CTS	input	Transfers data when on.
Data set ready	DSR	input	Not used.
Signal ground	SG	-	Used to ground signal
Data terminal ready	DTR	output	Always on.

(3) Signal Specifications

Signal status	Signal voltage
SPACE (ON)	+ 3 V or higher
MARK (OFF)	- 3 V or lower

Notes



**TOSOH CORPORATION
BIOSCIENCE DIVISION**

2-2-1 Yaesu, Chuo-ku
Tokyo 104-0028 Japan
Phone: +81 3 6636 3734
Fax: +81 3 6636 3627
Website: www.tosoh.com



TOSOH EUROPE N.V.

Transportstraat 4
3980 Tessenderlo-Ham, Belgium
Phone: +32 13 66 88 30
Fax: +32 13 66 47 49
Website: www.tosohbioscience.com



TOSOH BIOSCIENCE LIMITED

Lytchett House, 13 Freeland Park,
Wareham Road, Poole, Dorset, BH16 6FA, UK
Phone :+44 1527 592901
Fax :+44 1527 471680



TOSOH BIOSCIENCE SA

Ankerstrasse 24
8004 Zürich
Switzerland

Supplied by

TOSOH BIOSCIENCE, INC.

3600 Gantz Road
Grove City, OH 43123 USA
Phone: +1 650 615 4970
Fax: +1 650 615 0415
Website: www.tosohbioscience.com